


Data Path : Z:\HPCHEM1\BNA G\DATA\BG013017\
 Data File : BG025701.D
 Acq On : 30 Jan 2017 12:35
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 18:29:38 2017

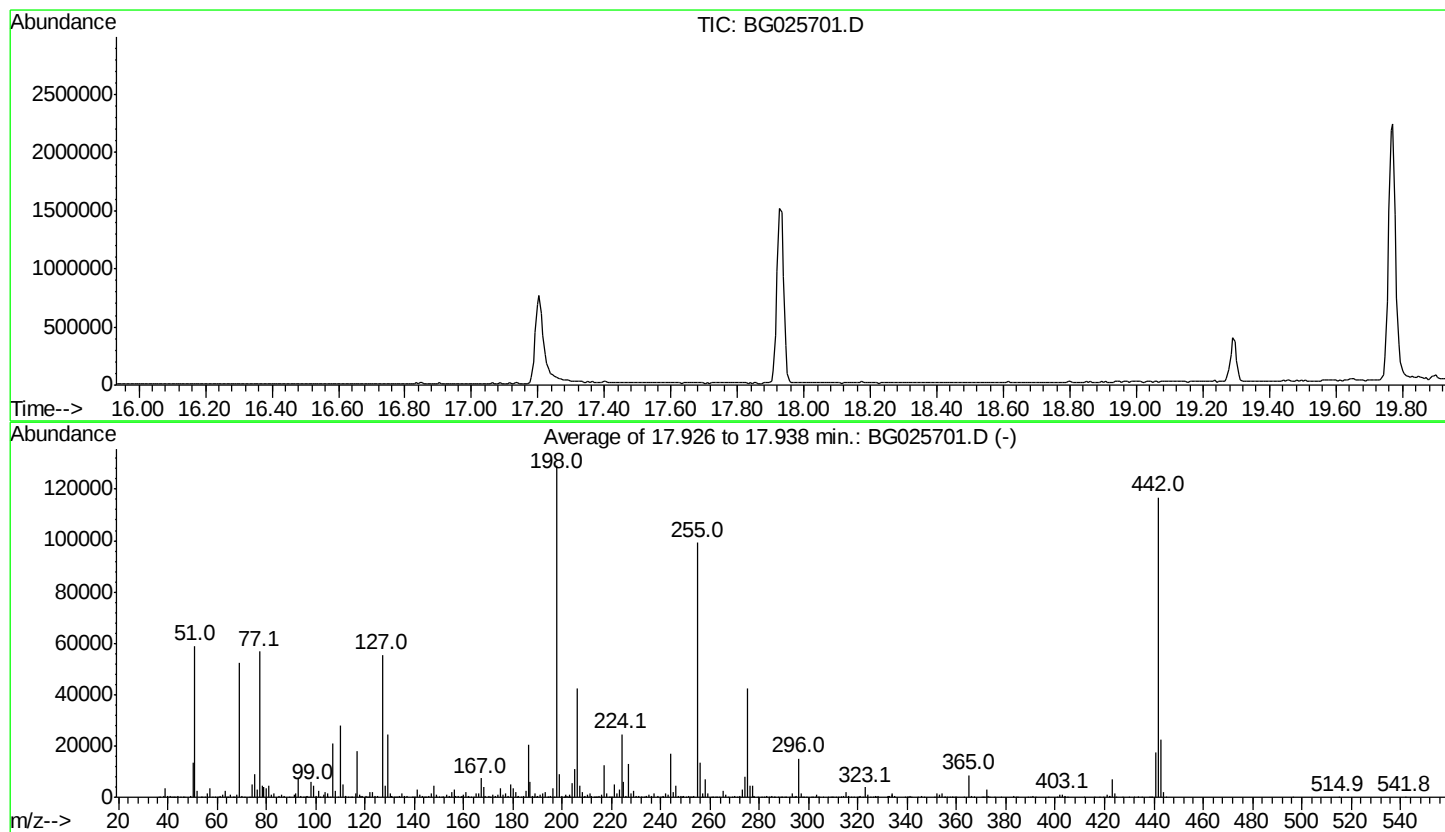

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	58921	PASS
68	69	0.00	2	1.5	803	PASS
69	198	0.00	100	40.6	52448	PASS
70	69	0.00	2	0.8	399	PASS
127	198	10	80	42.9	55370	PASS
197	198	0.00	2	0.2	267	PASS
198	198	100	100	100.0	129202	PASS
199	198	5	9	7.0	9106	PASS
275	198	10	60	32.9	42530	PASS
365	198	1	100	6.6	8566	PASS
441	442	0.01	24	15.1	17713	PASS
442	198	50	100	90.5	116938	PASS
443	442	15	24	19.2	22400	PASS