
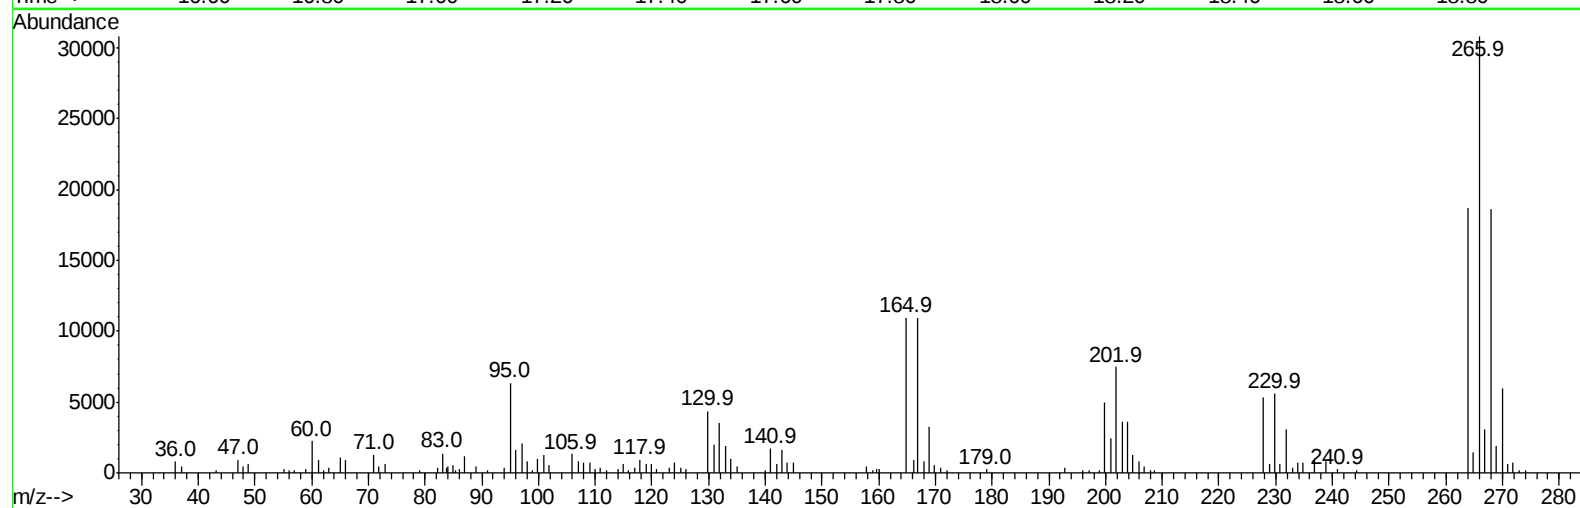


Data Path : U:\HPCHEM1\BNA G\DATA\BG013018\
Data File : BG032441.D
Acq On : 30 Jan 2018 14:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 04:30:31 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

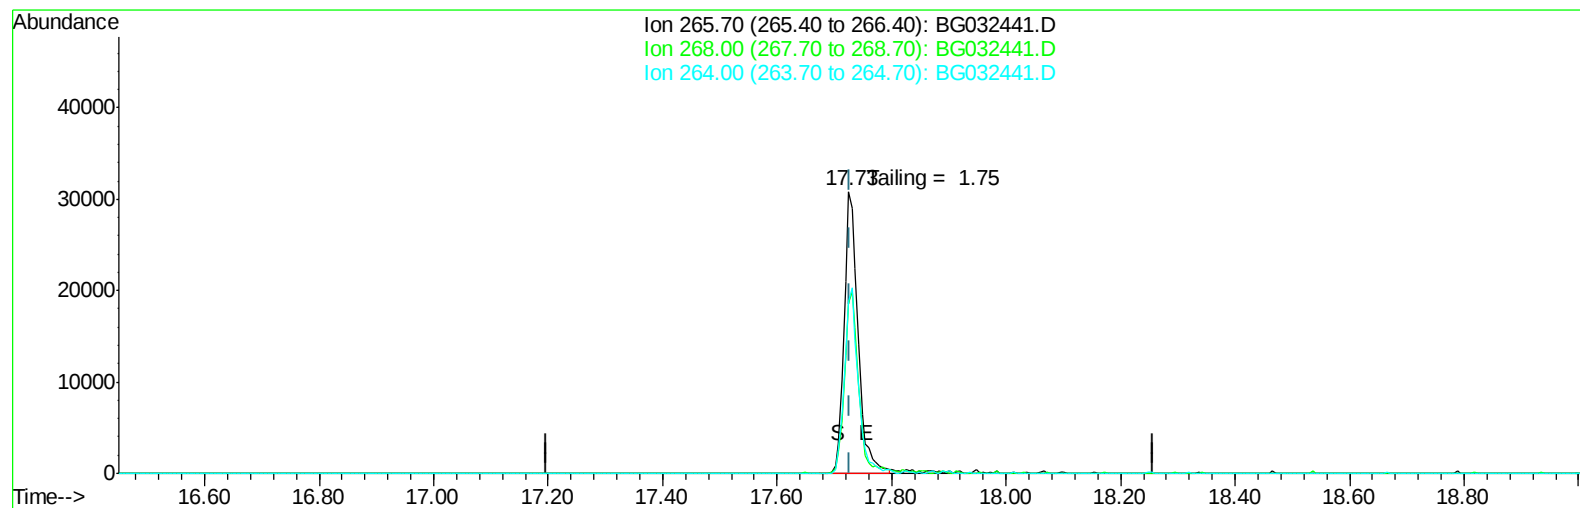

TIC: BG032441.D

(69) Pentachlorophenol (C)



17.725min (-0.004) 50672.84ng

response 53084

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.53
264.00	62.00	60.84
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG013018\
Data File : BG032441.D
Acq On : 30 Jan 2018 14:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 04:30:31 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

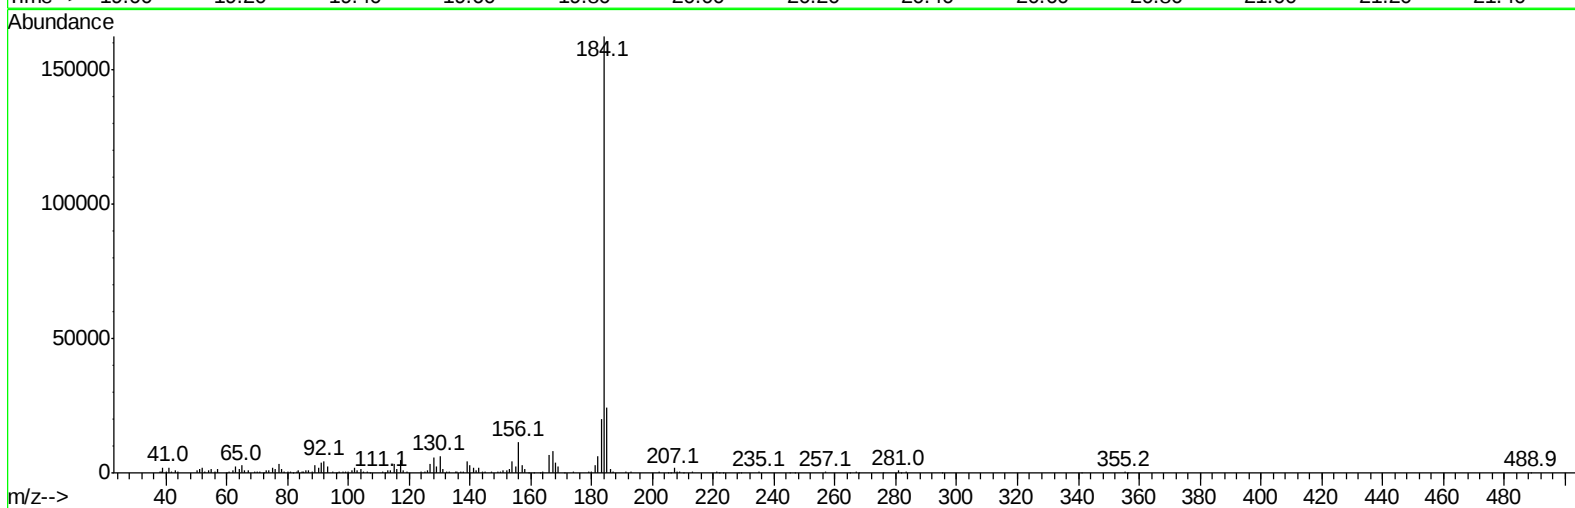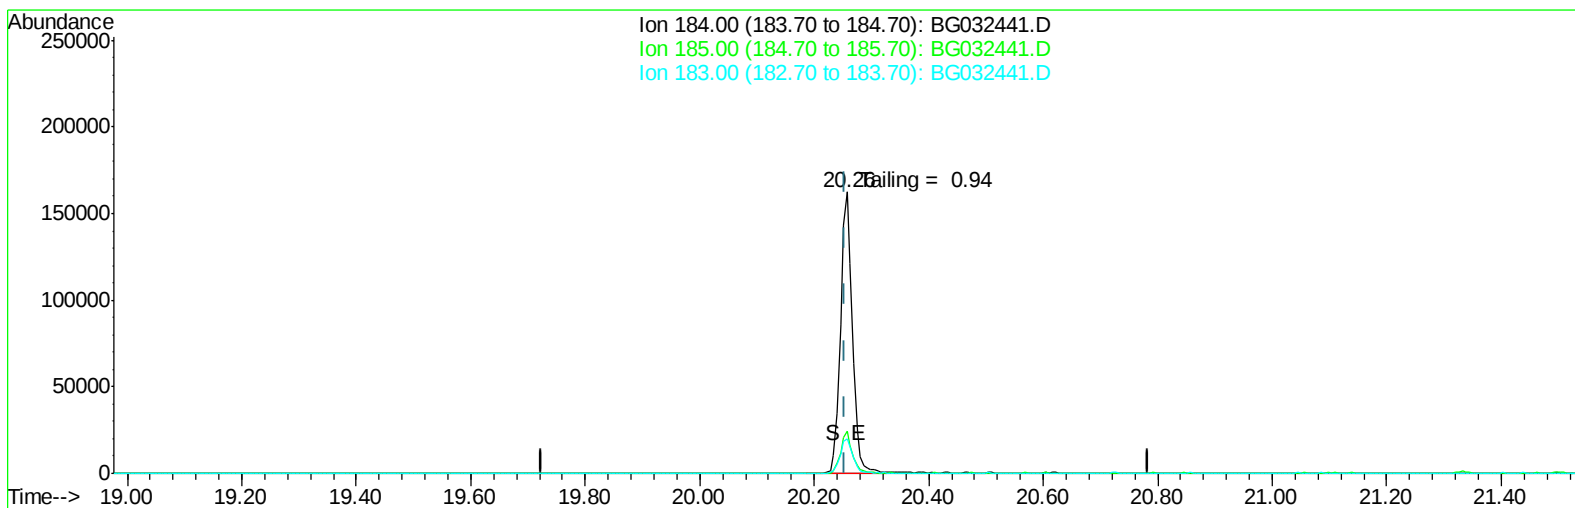

TIC: BG032441.D

(76) Benzidine

20.257min (+0.002) 615.02ng

response 238210

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.93
183.00	13.30	12.45
0.00	0.00	0.00