


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG013018\
 Data File : BG032441.D
 Acq On : 30 Jan 2018 14:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 29 15:32:55 2018

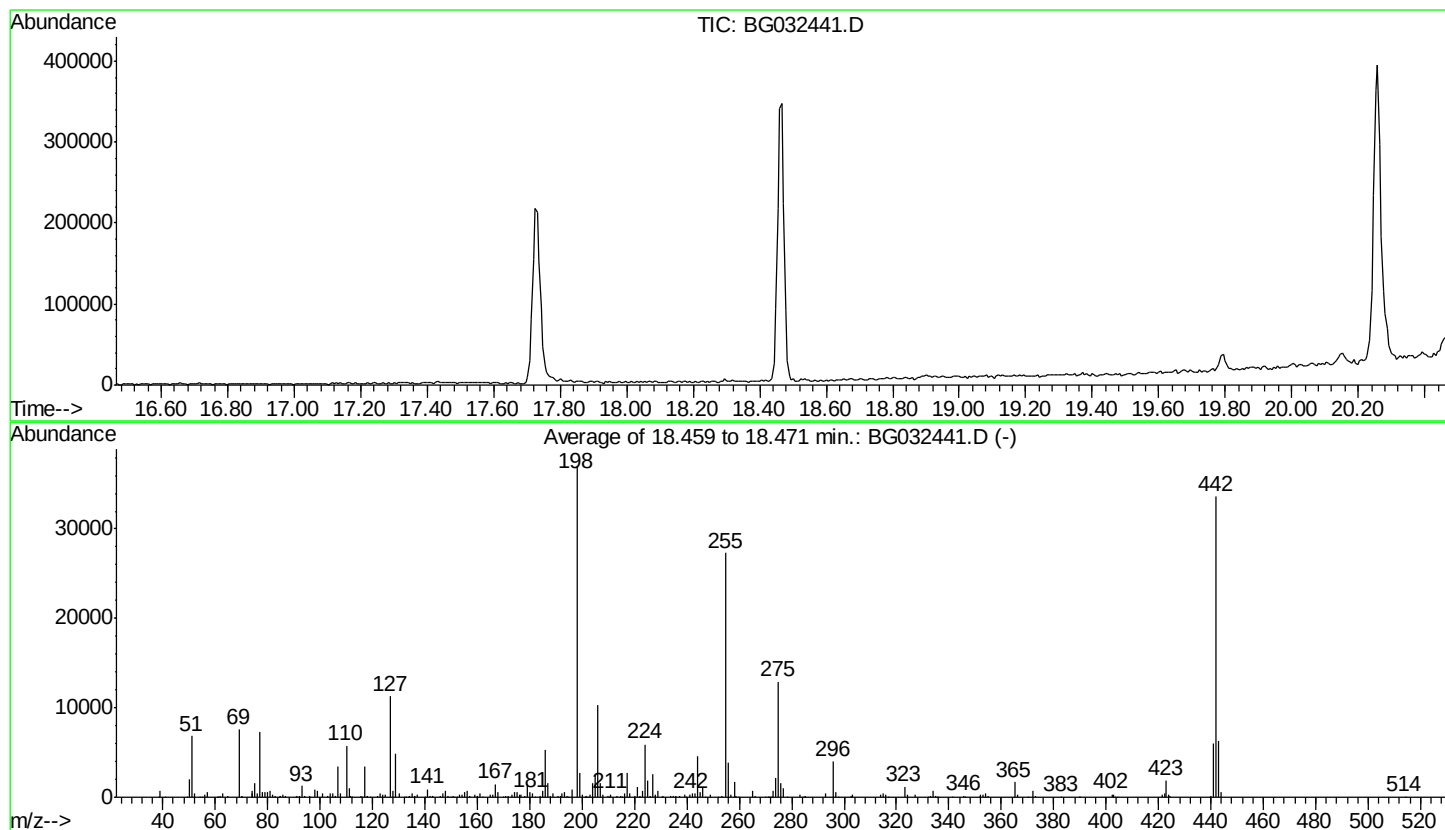

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.5	6860	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	20.3	7528	PASS
70	69	0.00	2	1.6	122	PASS
127	198	10	80	30.4	11271	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	37088	PASS
199	198	5	9	7.5	2777	PASS
275	198	10	60	34.8	12890	PASS
365	198	1	100	4.6	1703	PASS
441	442	0.01	24	17.9	6001	PASS
442	198	50	100	90.6	33600	PASS
443	442	15	24	18.6	6256	PASS