
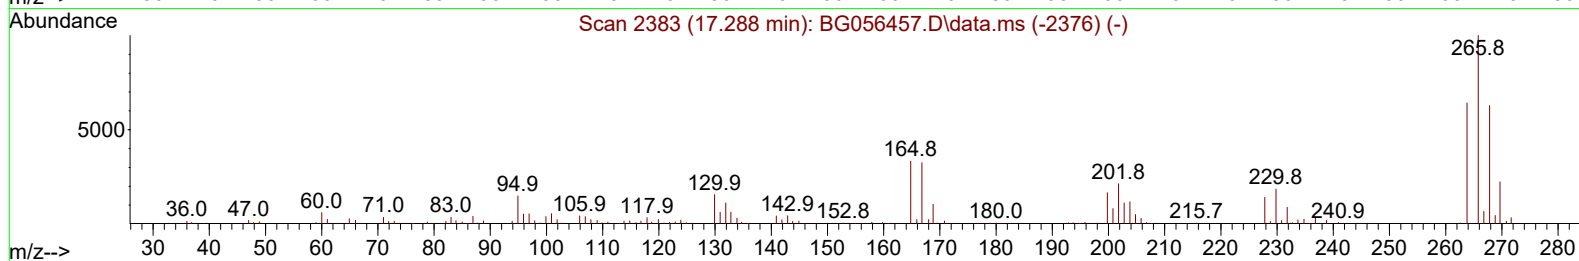
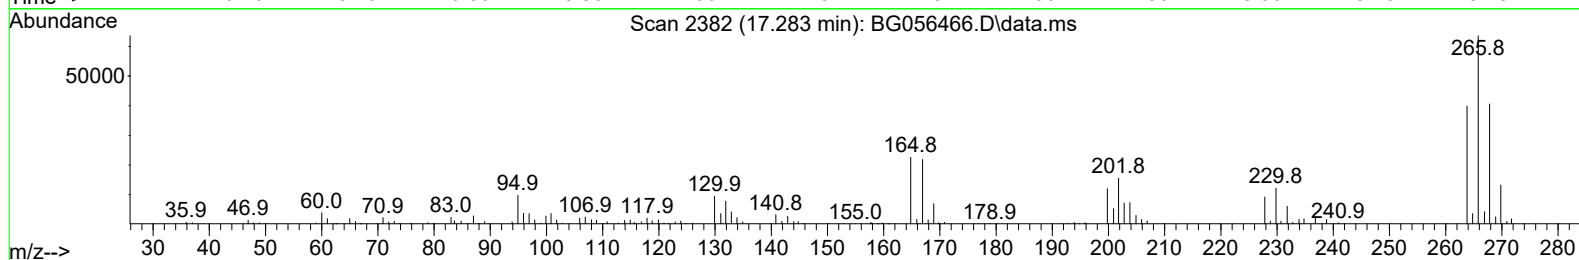


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013023\
Data File : BG056466.D
Acq On : 30 Jan 2023 9:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 06:19:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 00:39:13 2023
Response via : Initial Calibration

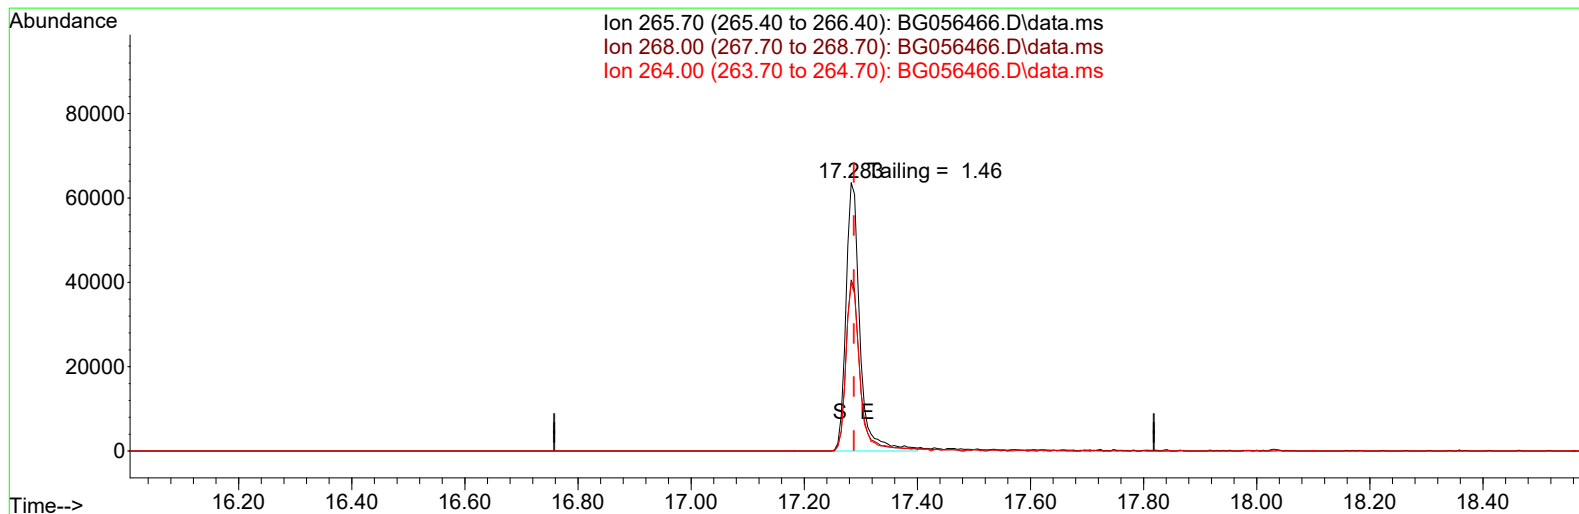

TIC: BG056466.D\data.ms

(70) Pentachlorophenol (C)




17.283min (-0.005) 24265.83 ng

response 107882

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	63.75
264.00	64.20	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013023\
 Data File : BG056466.D
 Acq On : 30 Jan 2023 9:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 06:19:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 28 00:39:13 2023
 Response via : Initial Calibration

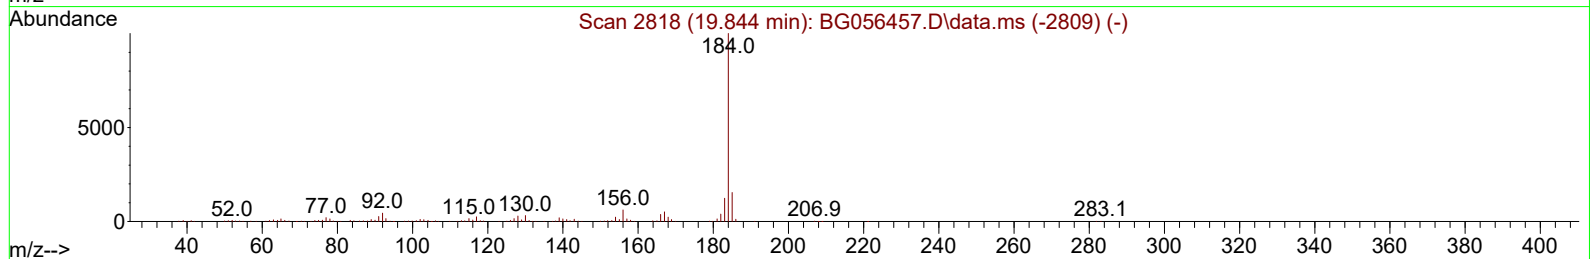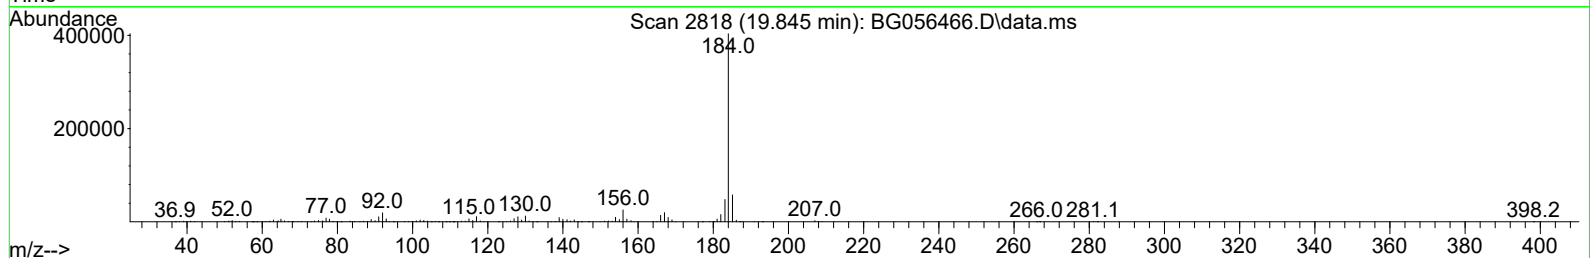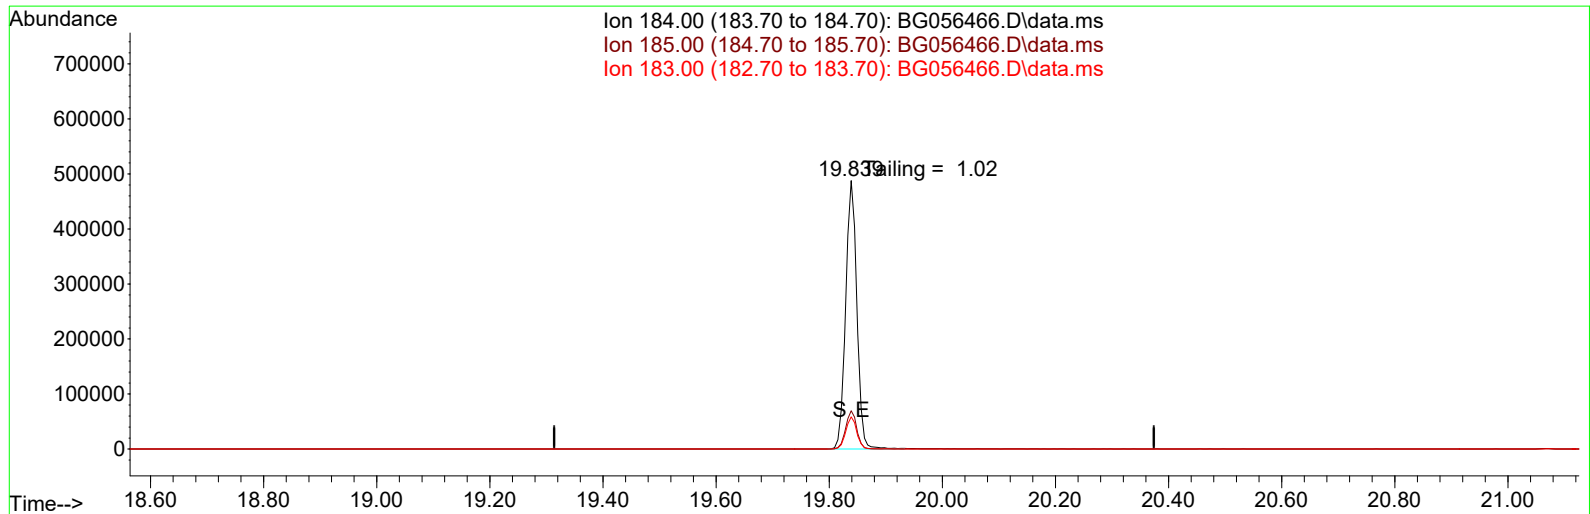

TIC: BG056466.D\data.ms

(77) Benzidine

19.844min (-19.844) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.40	0.00#
183.00	12.30	0.00#
0.00	0.00	0.00