
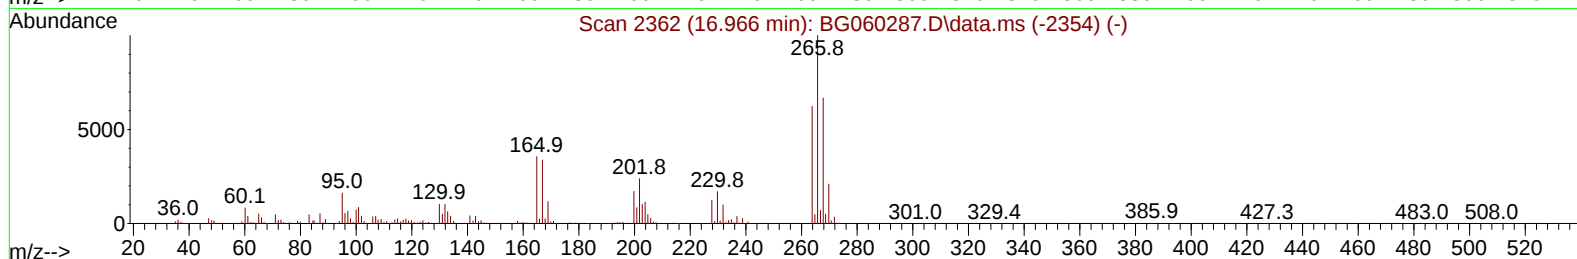
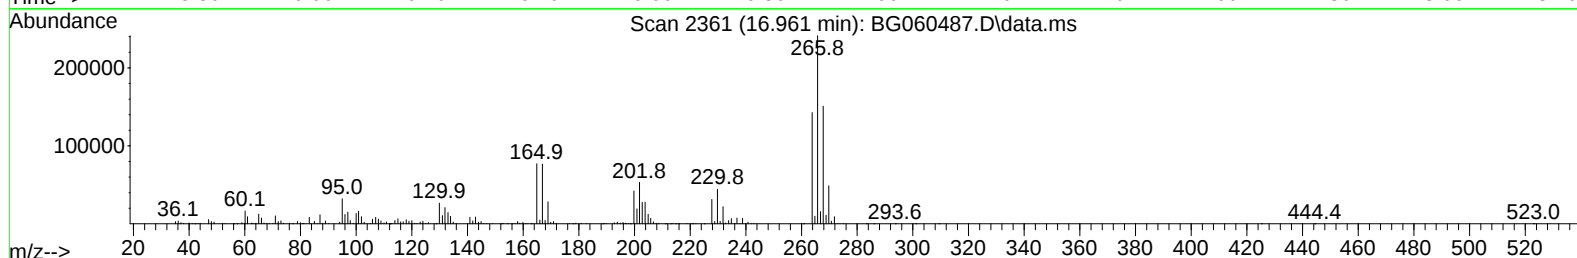


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013024\
Data File : BG060487.D
Acq On : 30 Jan 2024 17:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 17:56:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

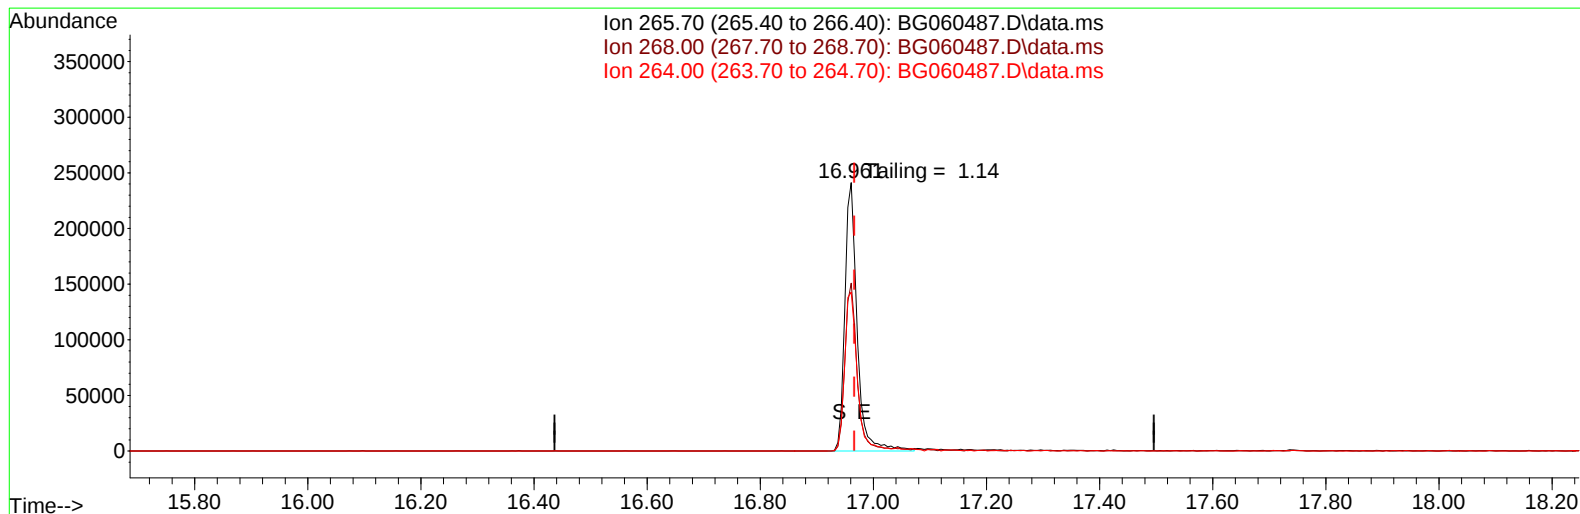

TIC: BG060487.D\data.ms

(70) Pentachlorophenol (C)




16.961min (-0.005) 854045.83 ng

response 365242

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	62.56
264.00	62.30	59.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013024\
Data File : BG060487.D
Acq On : 30 Jan 2024 17:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 17:56:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

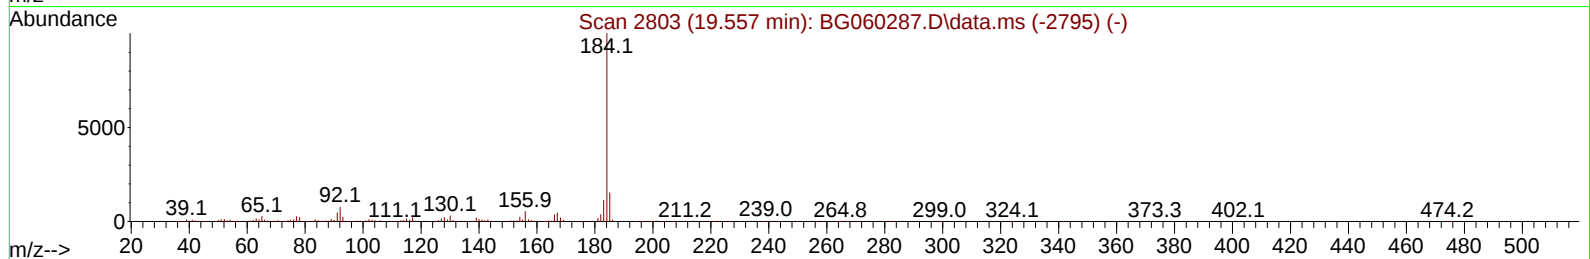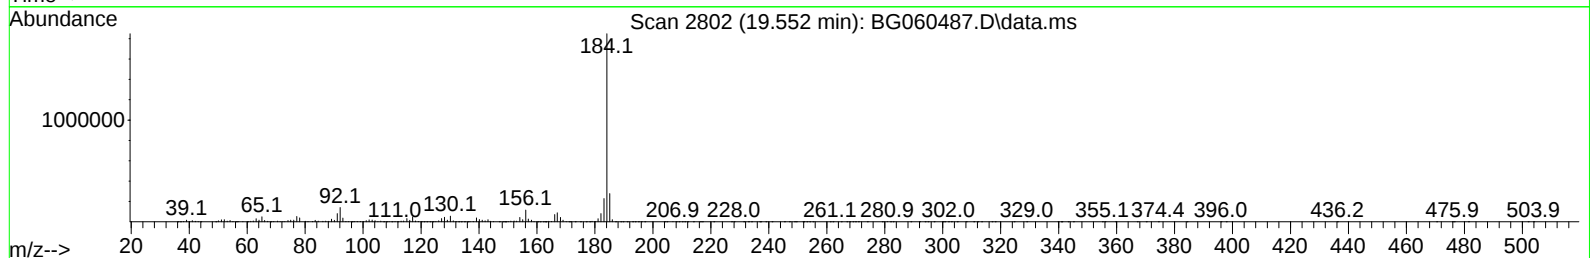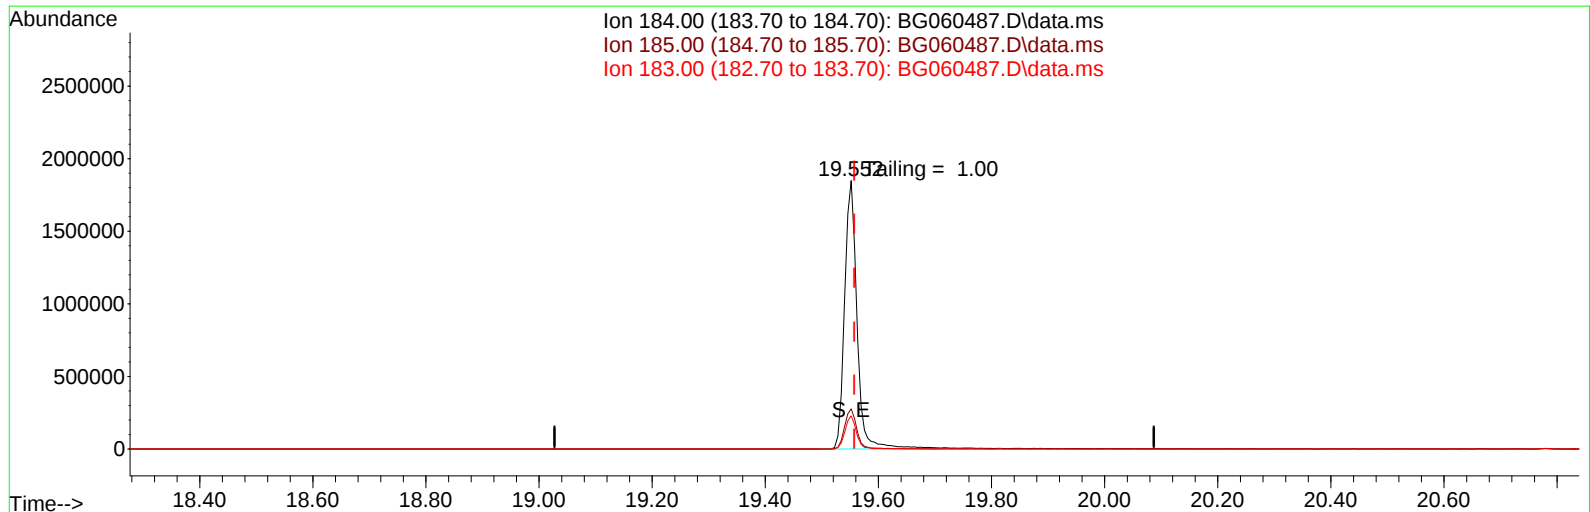

TIC: BG060487.D\data.ms

(77) Benzidine

19.552min (-0.005) 176076.65 ng

response 2830723

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.96
183.00	11.20	12.37
0.00	0.00	0.00