

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013024\
 Data File : BG060501.D
 Acq On : 31 Jan 2024 2:45
 Operator : MA/JU
 Sample : P1243-03 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MR-308-17-19

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060501.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.503	404	411	420	rBV	904056	1520744	34.10%	4.815%
2	7.095	674	682	698	rBV	973604	1761038	39.49%	5.575%
3	7.923	816	823	838	rBV	580613	1046535	23.47%	3.313%
4	9.087	1013	1021	1037	rBV	625817	1172869	26.30%	3.713%
5	10.726	1292	1300	1308	rBV	845857	1546637	34.68%	4.897%
6	13.182	1711	1718	1730	rBV	2062091	3261348	73.13%	10.325%
7	13.446	1759	1763	1771	rVB2	31184	52699	1.18%	0.167%
8	14.563	1939	1953	1960	rBV	1545063	2390683	53.61%	7.569%
9	15.614	2127	2132	2136	rBV2	30004	49304	1.11%	0.156%
10	16.055	2200	2207	2216	rBV	1478508	2284991	51.24%	7.234%
11	16.607	2296	2301	2307	rBV10	19252	47618	1.07%	0.151%
12	17.312	2415	2421	2425	rBV	1903677	2796257	62.70%	8.853%
13	17.354	2425	2428	2434	rVB	404009	573574	12.86%	1.816%
14	17.448	2439	2444	2448	rVB	82074	129733	2.91%	0.411%
15	18.194	2566	2571	2575	rBV3	125402	209968	4.71%	0.665%
16	18.235	2575	2578	2583	rVB	92218	130333	2.92%	0.413%
17	18.382	2599	2603	2607	rBV3	103636	186419	4.18%	0.590%
18	18.681	2652	2654	2659	rVB2	48601	59743	1.34%	0.189%
19	19.369	2766	2771	2777	rVB	797005	1108501	24.86%	3.510%
20	19.698	2824	2827	2828	rBV	96595	102881	2.31%	0.326%
21	19.733	2829	2833	2839	rVB	761896	1055369	23.67%	3.341%
22	19.927	2861	2866	2872	rBV	3449354	4459583	100.00%	14.119%
23	21.578	3140	3147	3152	rBV2	1714100	3384080	75.88%	10.714%
24	24.751	3680	3687	3701	rVB2	806979	2254642	50.56%	7.138%




Sum of corrected areas: 31585549

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013024\
Data File : BG060501.D
Acq On : 31 Jan 2024 2:45
Operator : MA/JU
Sample : P1243-03 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MR-308-17-19

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

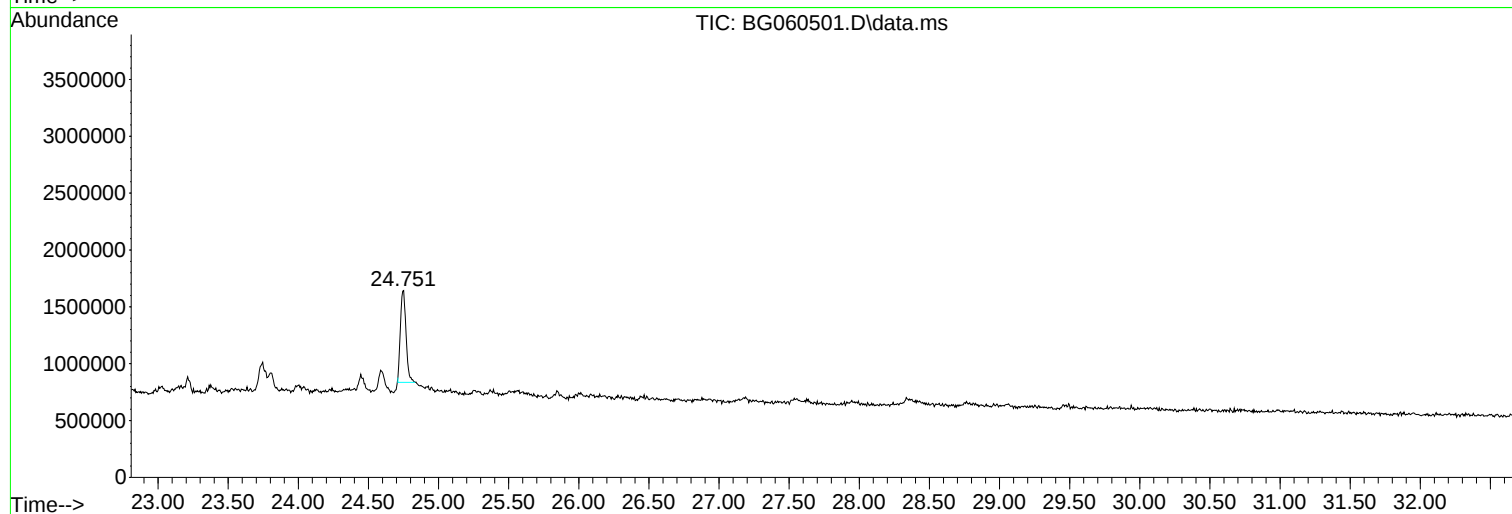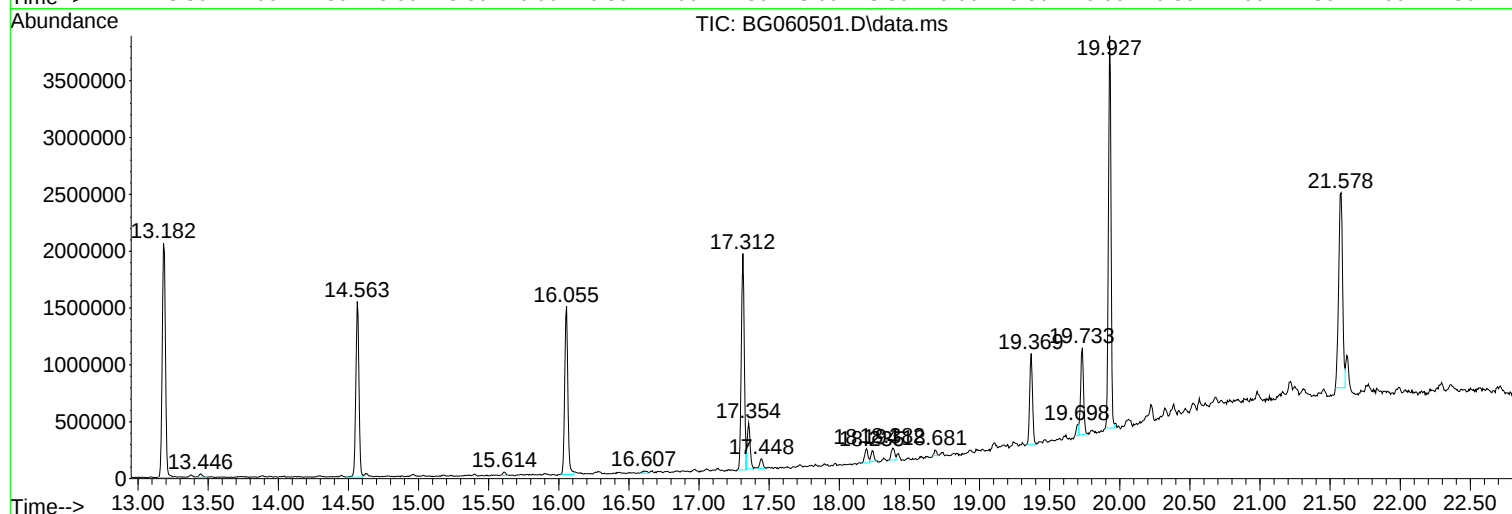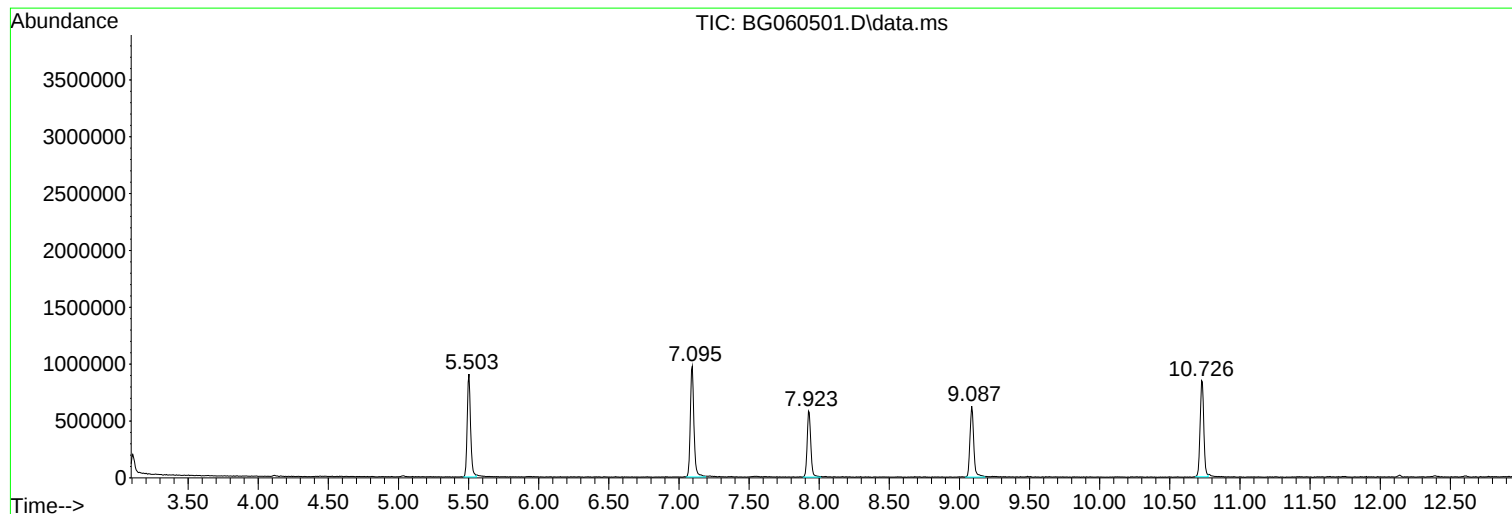

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013024\
Data File : BG060501.D
Acq On : 31 Jan 2024 2:45
Operator : MA/JU
Sample : P1243-03 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MR-308-17-19

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013024\
Data File : BG060501.D
Acq On : 31 Jan 2024 2:45
Operator : MA/JU
Sample : P1243-03 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MR-308-17-19

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------