


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013024\
Data File : BG060477.D
Acq On : 30 Jan 2024 10:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

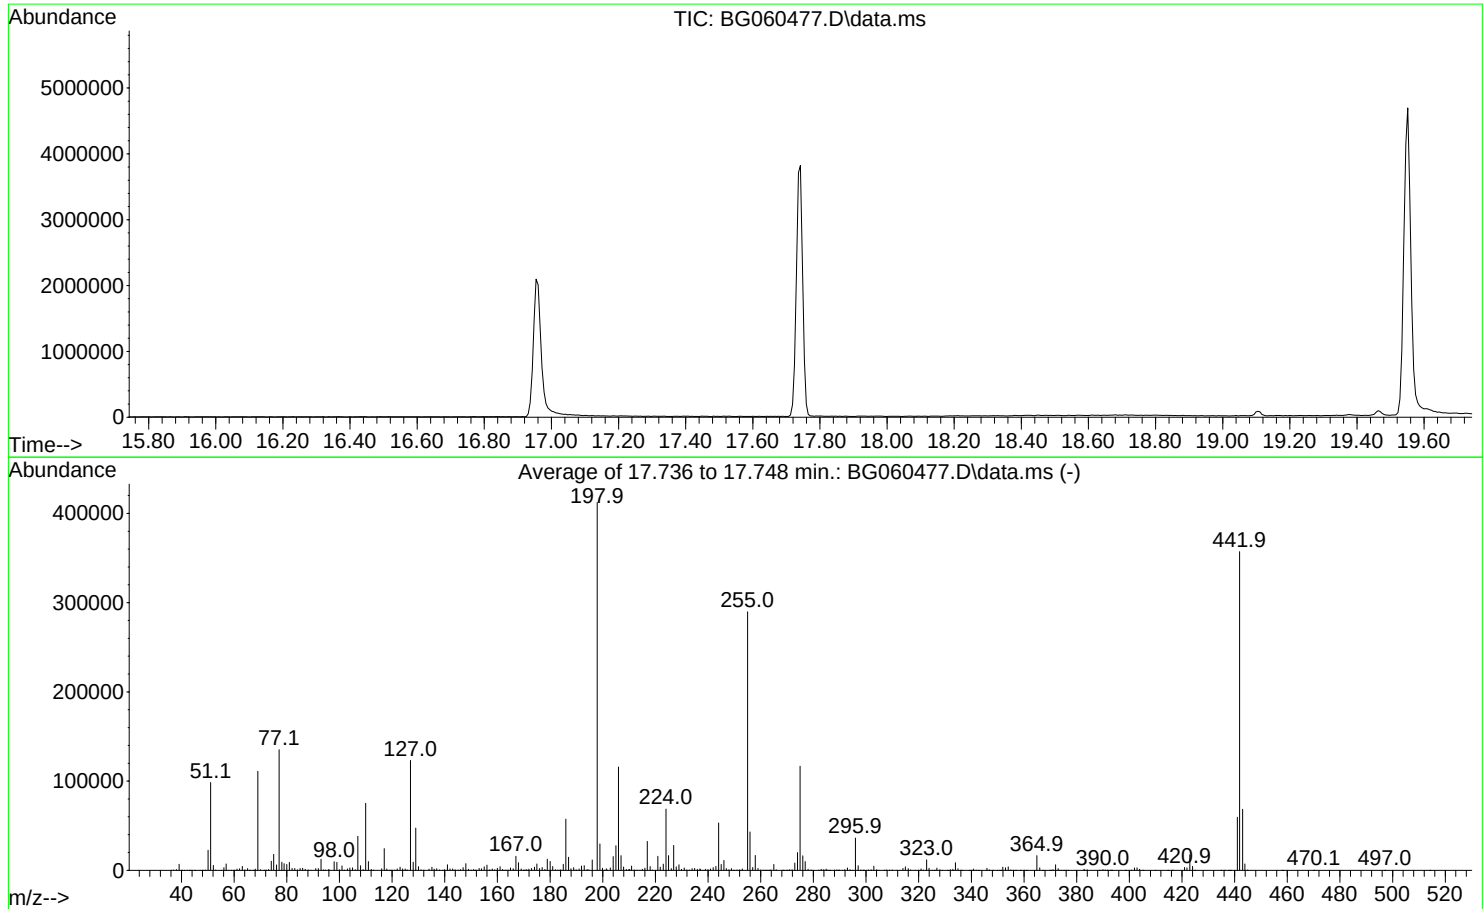




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.9	98357	PASS
68	69	0.00	2	1.4	1516	PASS
69	198	0.00	100	26.9	111048	PASS
70	69	0.00	2	0.6	674	PASS
127	198	10	80	29.9	123141	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	412203	PASS
199	198	5	9	7.2	29672	PASS
275	198	10	60	28.3	116699	PASS
365	198	1	100	4.0	16433	PASS
441	198	0.01	100	14.4	59552	PASS
442	442	50	100	100.0	357163	PASS
443	442	15	24	19.2	68424	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013024\
Data File : BG060477.D
Acq On : 30 Jan 2024 10:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 30 12:02:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

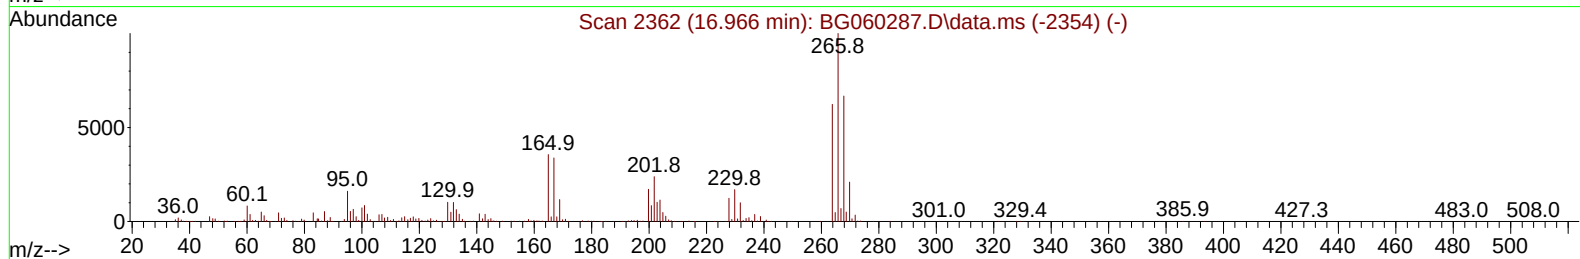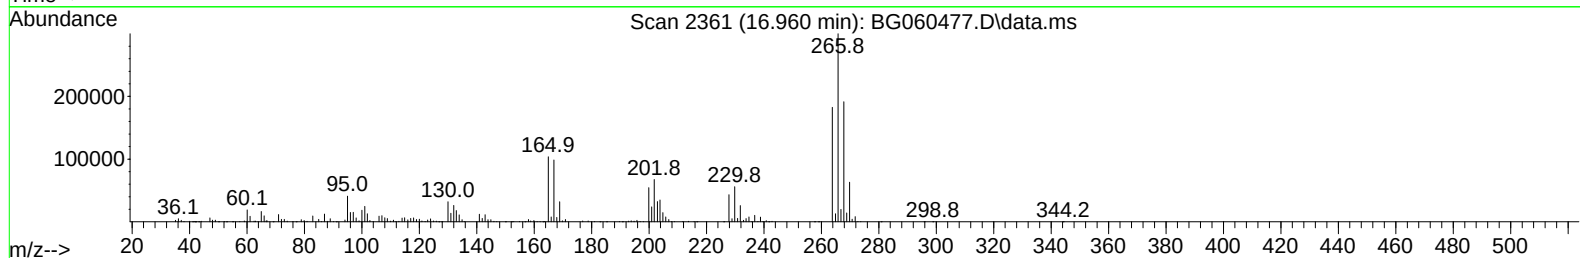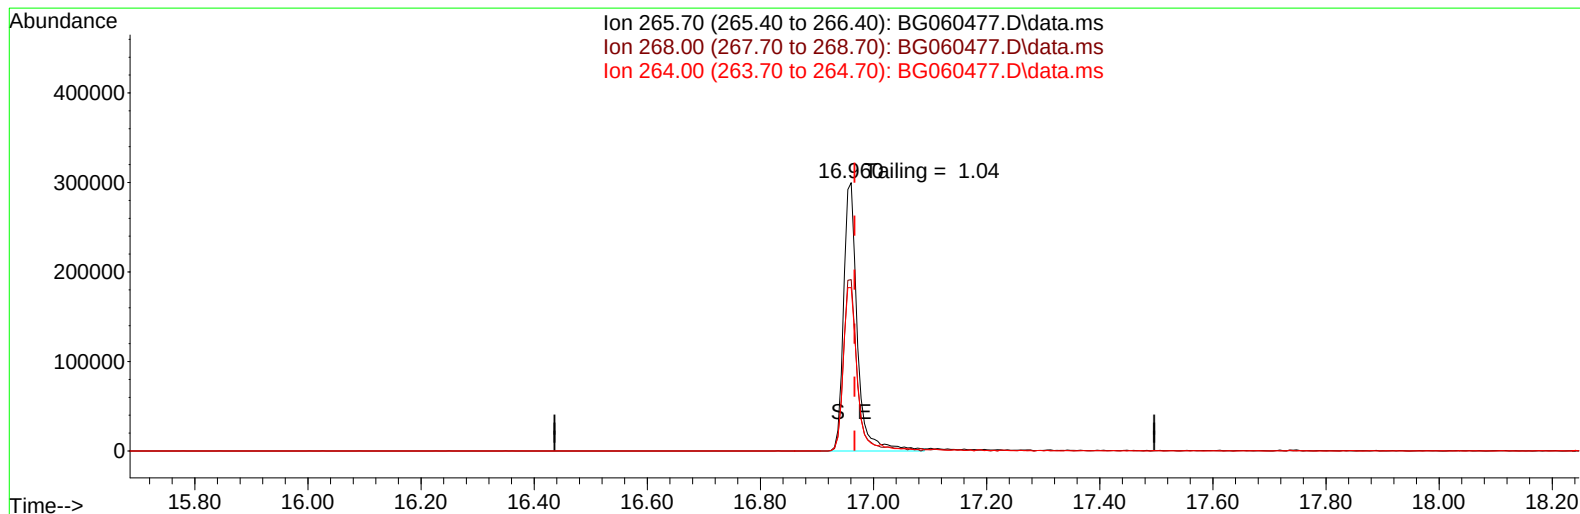

TIC: BG060477.D\data.ms

(70) Pentachlorophenol (C)

16.960min (-0.006) 616099.70 ng




response 509686

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	63.86
264.00	62.30	60.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013024\
Data File : BG060477.D
Acq On : 30 Jan 2024 10:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 30 12:02:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

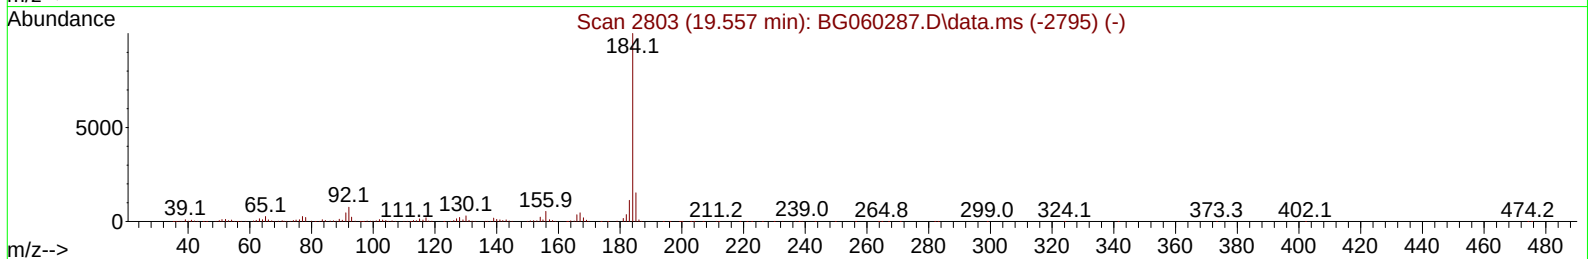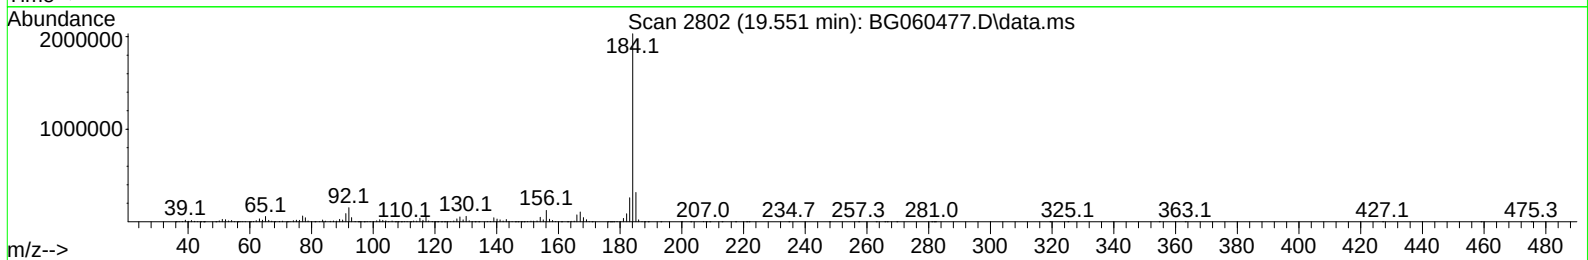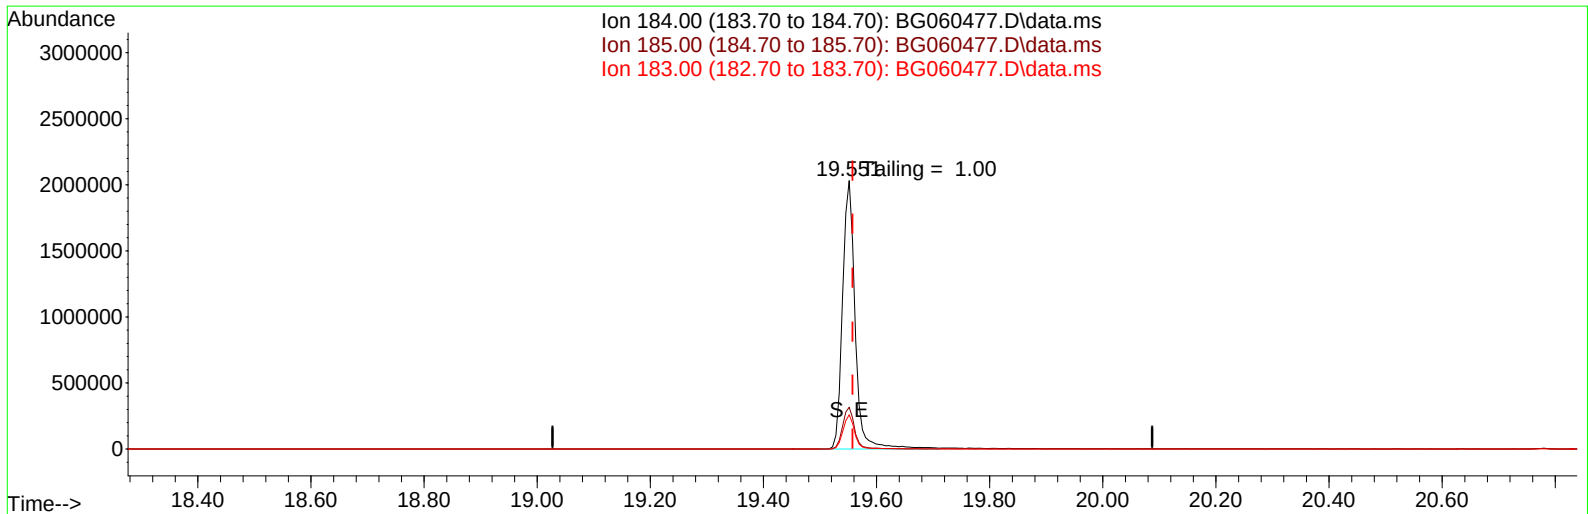

TIC: BG060477.D\data.ms

(77) Benzidine

19.551min (-0.006) 1646802.13 ng m

response 3148386

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	15.58
183.00	11.20	12.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/30/2024	BNA_G	<u>BG060477.D</u>
Compound Name	Response	Retention Time
DDT	1580375	20.779
DDD	25089	20.386
DDE	1522	19.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26611	1606986	1.66

Instrument :
BNA_G
ClientSampleId :
DFTPP