


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013024\
Data File : BG060487.D
Acq On : 30 Jan 2024 17:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

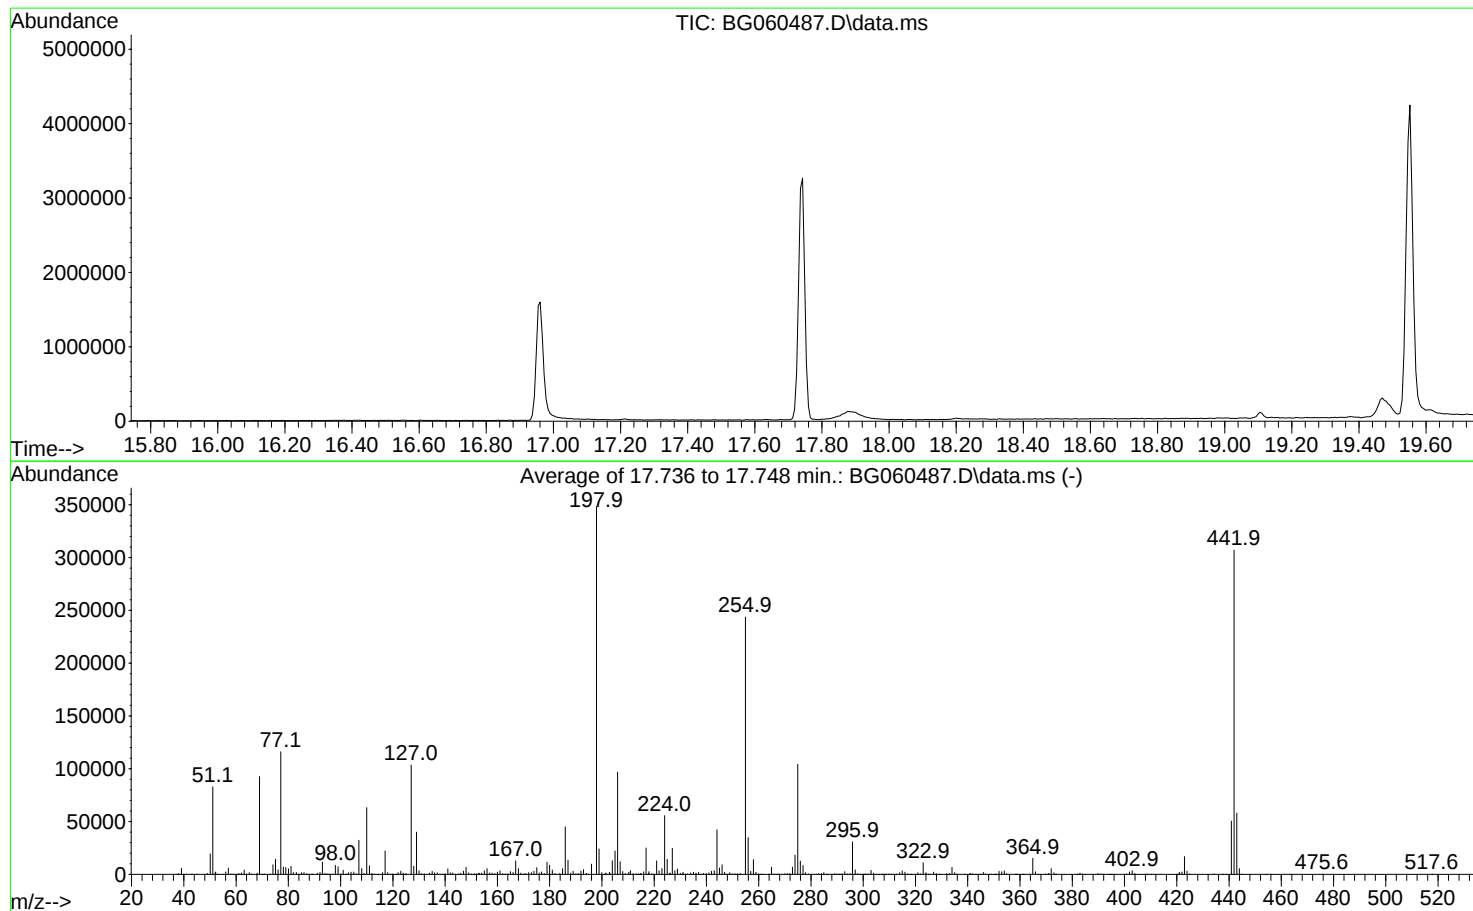




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.8	82859	PASS
68	69	0.00	2	1.3	1188	PASS
69	198	0.00	100	26.6	92590	PASS
70	69	0.00	2	0.4	330	PASS
127	198	10	80	29.7	103461	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	348309	PASS
199	198	5	9	6.9	24149	PASS
275	198	10	60	29.9	104256	PASS
365	198	1	100	4.3	15097	PASS
441	198	0.01	100	14.5	50445	PASS
442	442	50	100	100.0	306987	PASS
443	442	15	24	18.9	58075	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013024\
Data File : BG060487.D
Acq On : 30 Jan 2024 17:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 30 17:56:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

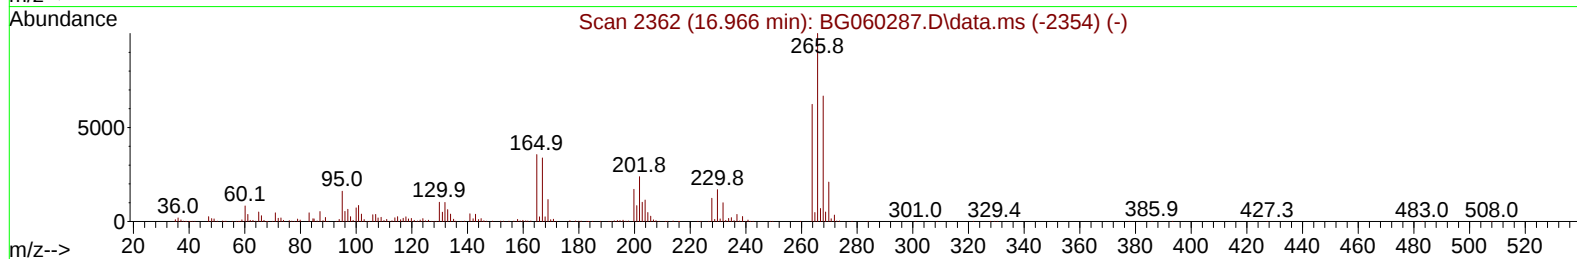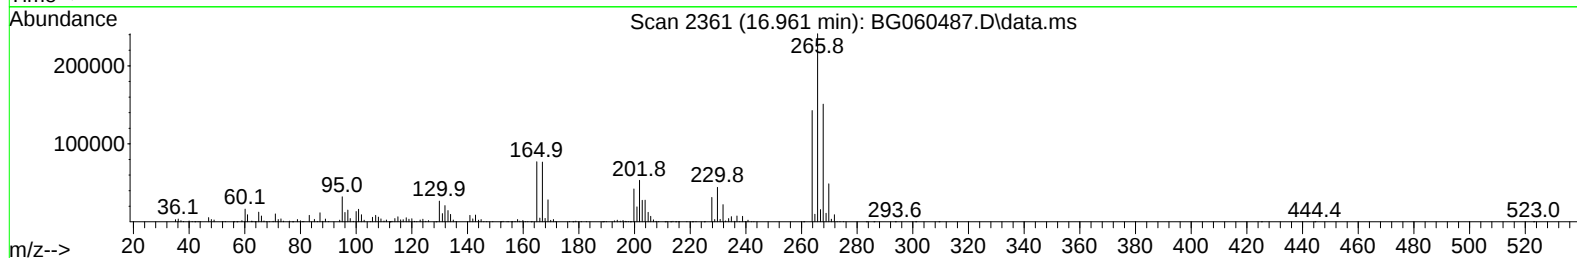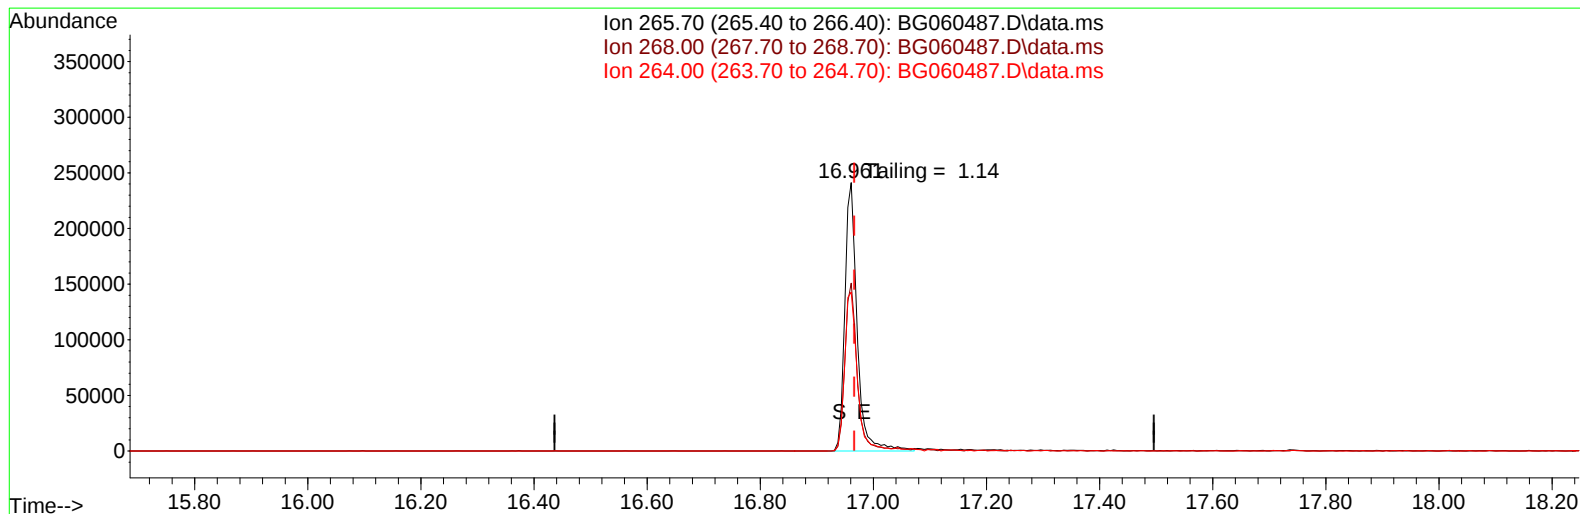

TIC: BG060487.D\data.ms

(70) Pentachlorophenol (C)

16.961min (-0.005) 854045.83 ng




response 365242

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	62.56
264.00	62.30	59.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013024\
Data File : BG060487.D
Acq On : 30 Jan 2024 17:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 30 17:56:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

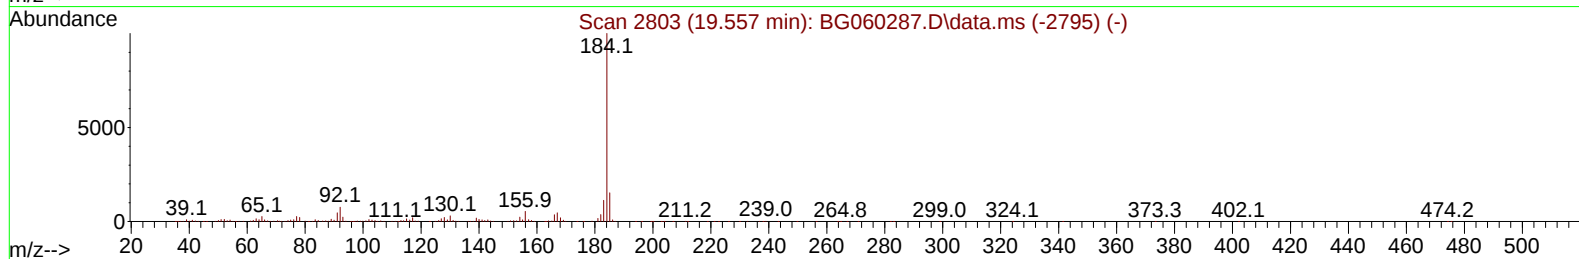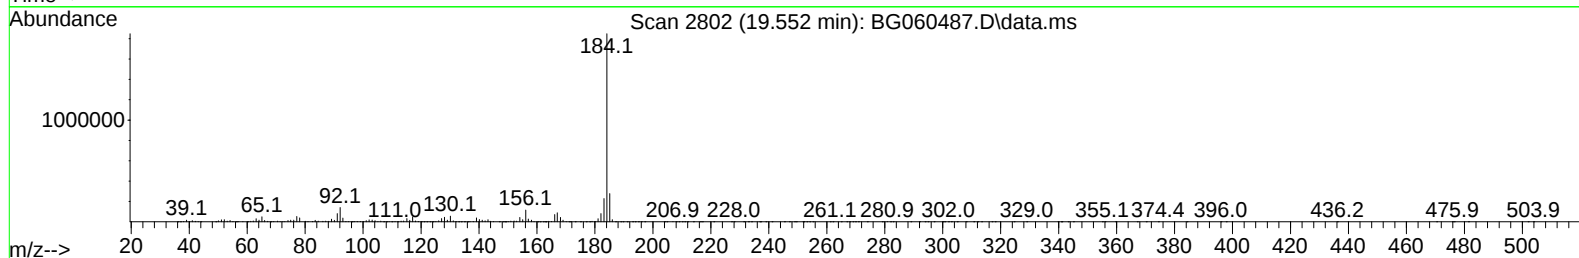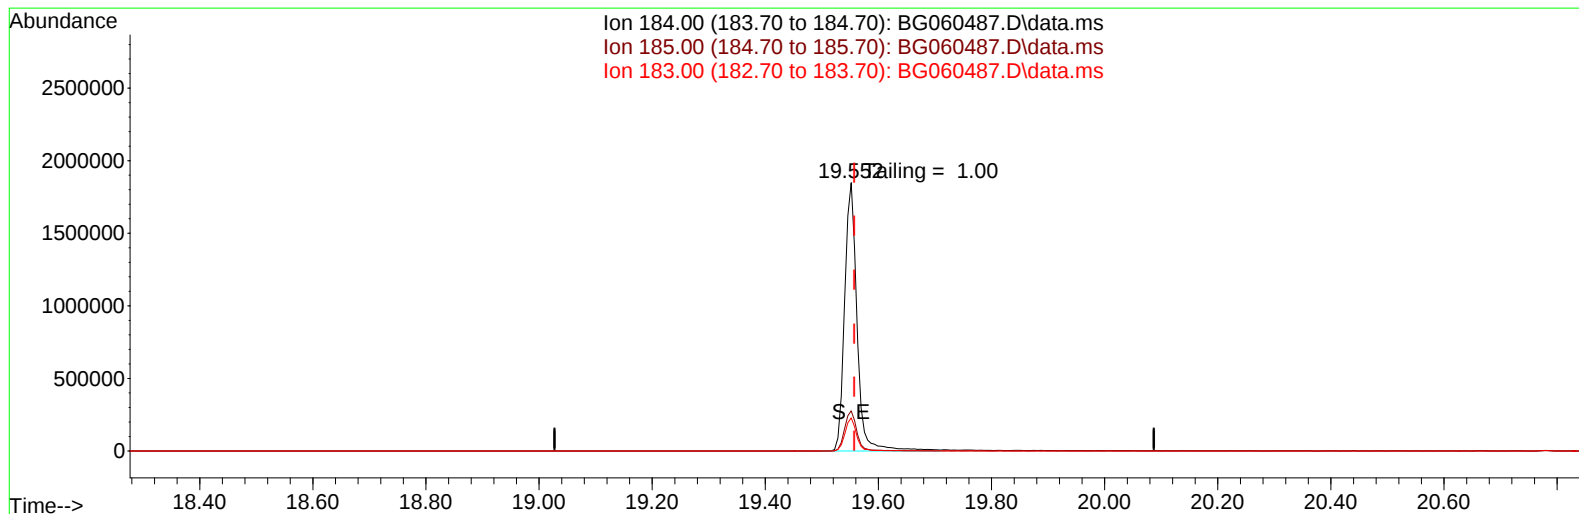

TIC: BG060487.D\data.ms

(77) Benzidine

19.552min (-0.005) 176076.65 ng

response 2830723

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.96
183.00	11.20	12.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/30/2024	BNA_G	<u>BG060487.D</u>
Compound Name	Response	Retention Time
DDT	1410613	20.78
DDD	33540	20.339
DDE	1517	19.834
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
35057	1445670	2.42

Instrument :
BNA_G
ClientSampleId :
DFTPP