
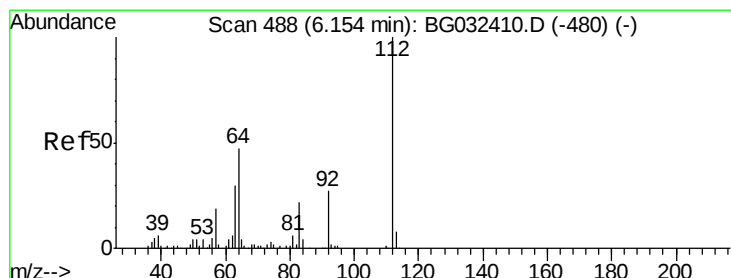
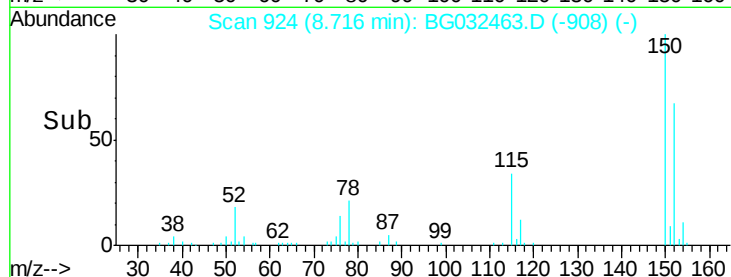
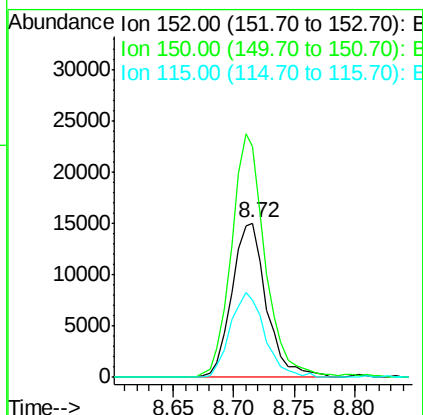


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.72 min Scan# 924
Delta R.T. -0.01 min
Lab File: BG032463.D
Acq: 31 Jan 2018 13:36

Instrument :
BNA_G
ClientSampleId :

Tgt Ion:152 Resp: 30059
Ion Ratio Lower Upper
152 100
150 149.0 126.6 189.8
115 50.4 53.0 79.4#

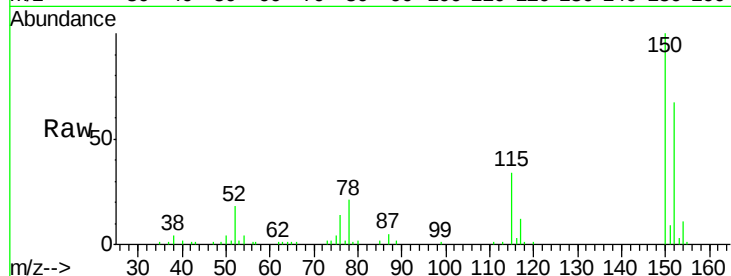

#5

2-Fluorophenol
Concen: 129.928 ng
RT: 6.15 min Scan# 488
Delta R.T. 0.00 min
Lab File: BG032463.D
Acq: 31 Jan 2018 13:36

Tgt Ion:112 Resp: 194443
Ion Ratio Lower Upper
112 100
64 49.6 56.3 84.5#
63 30.2 30.1 45.1

