
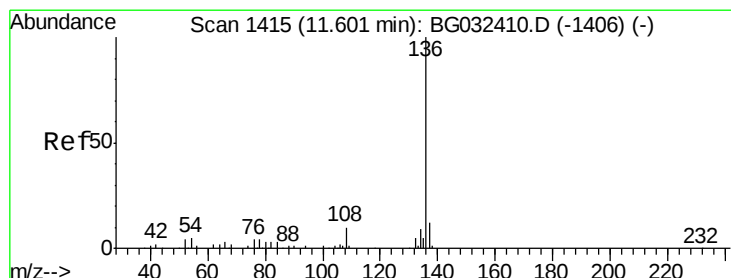
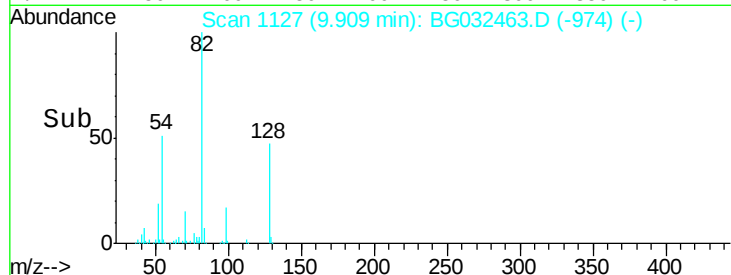
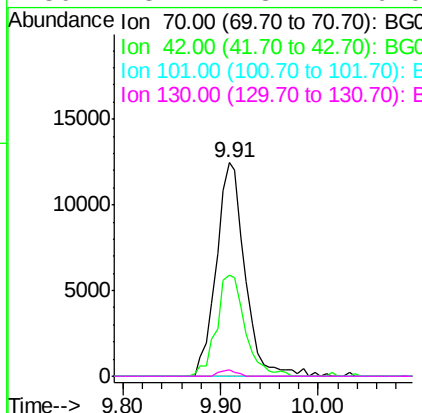


#19
 n-Nitroso-di-n-propylamine
 Concen: 19.085 ng
 RT: 9.91 min Scan# 1127
 Delta R.T. 0.37 min
 Lab File: BG032463.D
 Acq: 31 Jan 2018 13:36

Instrument :
 BNA_G
 ClientSampleId :

Tgt Ion: 70 Resp: 25271
 Ion Ratio Lower Upper
 70 100
 42 47.3 49.1 73.7#
 101 0.0 8.5 12.7#
 130 3.2 13.4 20.0#

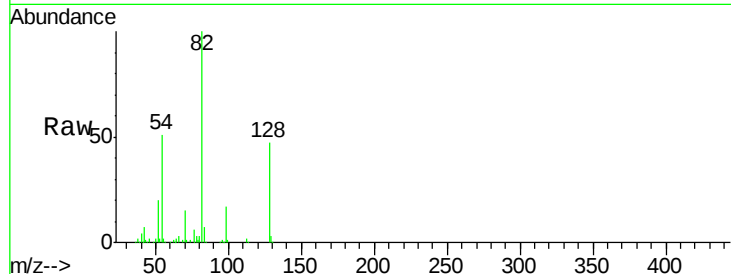

#21
 Naphthalene-d8
 Concen: 20.000 ng
 RT: 11.59 min Scan# 1413
 Delta R.T. -0.01 min
 Lab File: BG032463.D
 Acq: 31 Jan 2018 13:36

Tgt Ion: 136 Resp: 117419
 Ion Ratio Lower Upper
 136 100
 137 10.1 9.2 13.8
 54 5.4 10.3 15.5#
 68 2.6 4.5 6.7#

