

#23

Nitrobenzene-d5

Concen: 88.953 ng

RT: 9.91 min Scan# 1127

Delta R.T. -0.01 min

Lab File: BG032463.D

Acq: 31 Jan 2018 13:36

Instrument :

BNA_G

ClientSampleId :


Tgt Ion: 82 Resp: 167222

Ion Ratio Lower Upper




82 100

128 46.6 29.7 44.5#

54 50.6 43.1 64.7

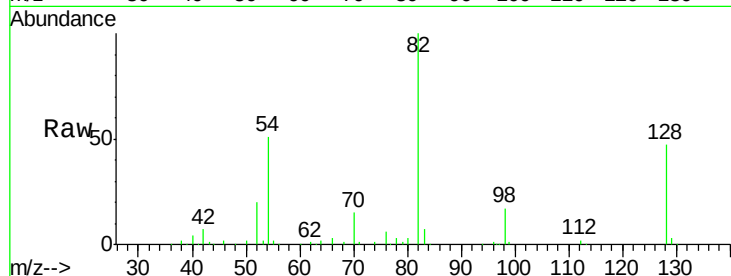

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

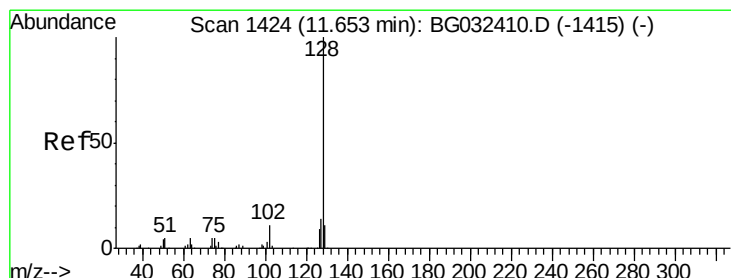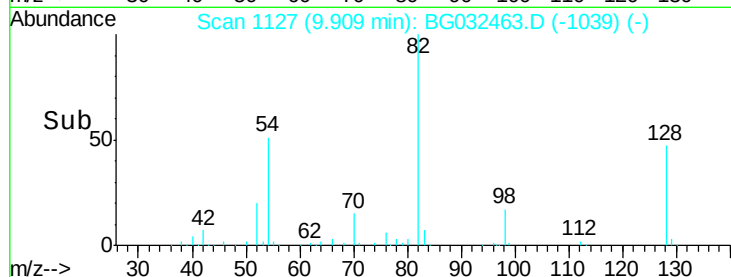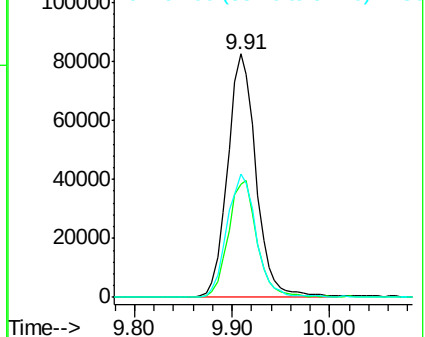

#31

Naphthalene

Concen: 3.048 ng

RT: 11.64 min Scan# 1422

Delta R.T. -0.01 min

Lab File: BG032463.D

Acq: 31 Jan 2018 13:36


Tgt Ion: 128 Resp: 17478

Ion Ratio Lower Upper

128 100

129 10.5 8.6 12.8

127 15.8 11.6 17.4

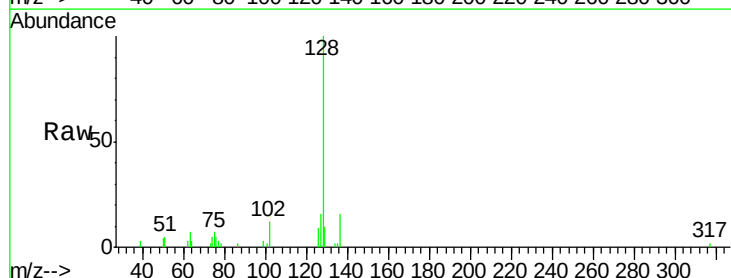

Abundance Ion 128.00 (127.70 to 128.70): BGC
Ion 129.00 (128.70 to 129.70): BGC
Ion 127.00 (126.70 to 127.70): BGC

