
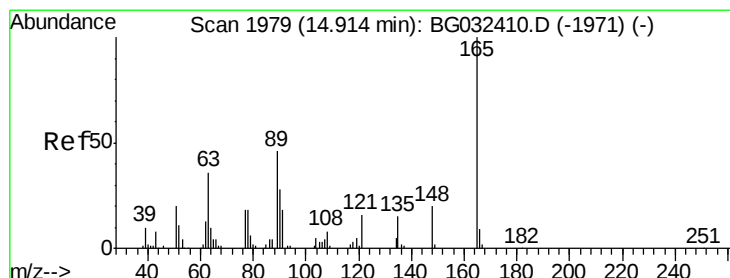
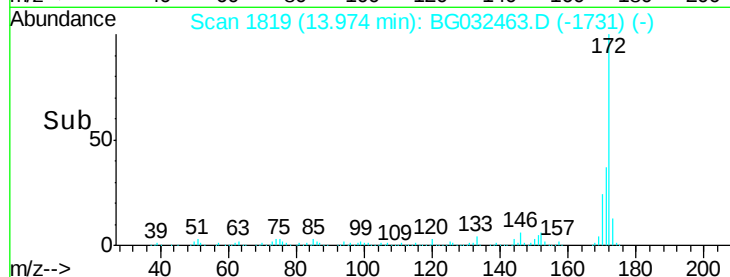
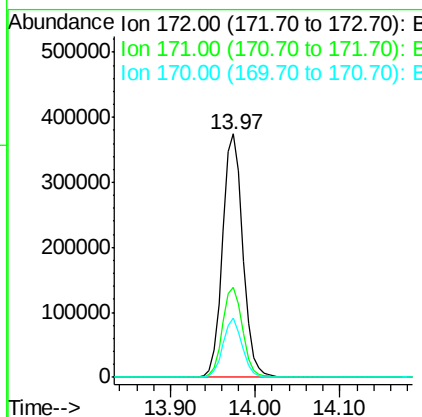


#44
 2-Fluorobiphenyl
 Concen: 93.401 ng
 RT: 13.97 min Scan# 1819
 Delta R.T. -0.01 min
 Lab File: BG032463.D
 Acq: 31 Jan 2018 13:36

Instrument :
 BNA_G
 ClientSampled :

Tgt Ion:172 Resp: 621121
 Ion Ratio Lower Upper
 172 100
 171 37.0 30.0 45.0
 170 24.2 19.5 29.3

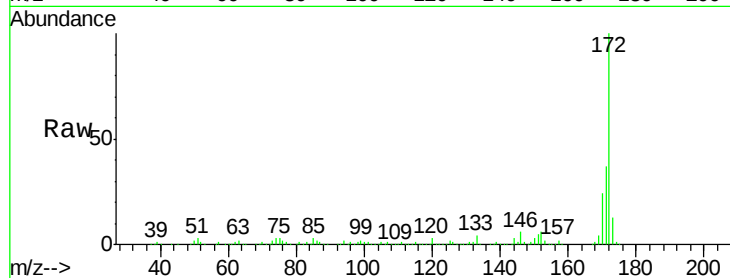

#50
 2,6-Dinitrotoluene
 Concen: 6.677 ng
 RT: 15.34 min Scan# 2052
 Delta R.T. 0.43 min
 Lab File: BG032463.D
 Acq: 31 Jan 2018 13:36

Tgt Ion:165 Resp: 10214
 Ion Ratio Lower Upper
 165 100
 63 0.0 52.7 79.1#
 89 3.0 49.2 73.8#

