
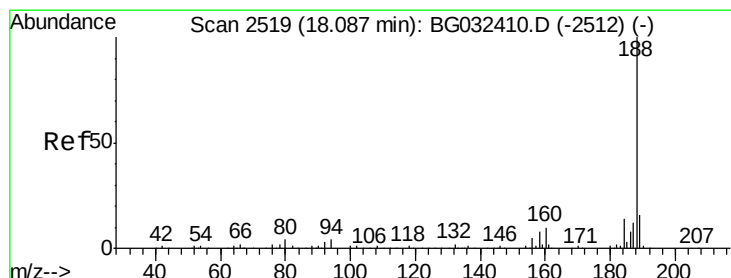
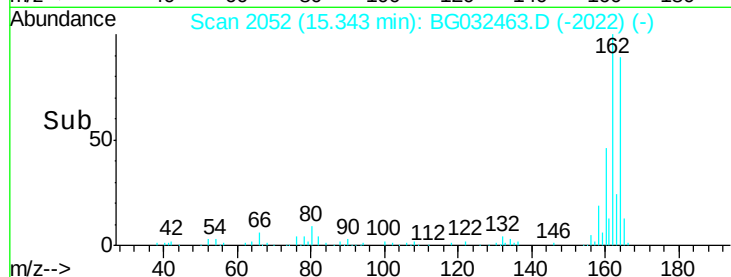
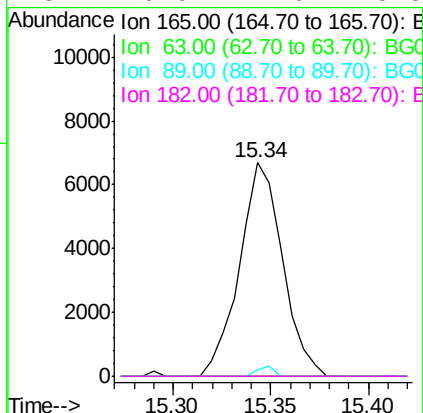


#56
 2,4-Dinitrotoluene
 Concen: 4.690 ng
 RT: 15.34 min Scan# 2052
 Delta R.T. -0.35 min
 Lab File: BG032463.D
 Acq: 31 Jan 2018 13:36

Instrument :
 BNA_G
 ClientSampleId :

Tgt Ion:165 Resp: 10214
 Ion Ratio Lower Upper
 165 100
 63 0.0 42.0 63.0#
 89 3.0 66.9 100.3#
 182 0.0 2.6 3.8#

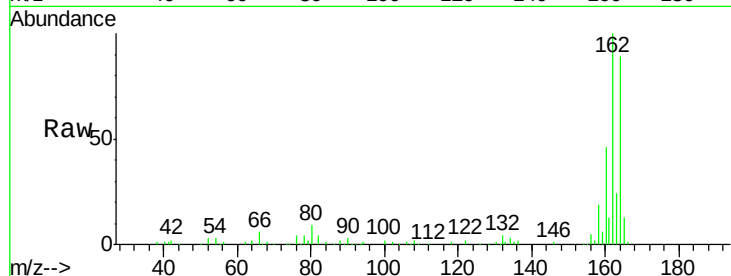

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 18.08 min Scan# 2518
 Delta R.T. -0.01 min
 Lab File: BG032463.D
 Acq: 31 Jan 2018 13:36

Tgt Ion:188 Resp: 216954
 Ion Ratio Lower Upper
 188 100
 94 4.0 6.9 10.3#
 80 4.1 7.7 11.5#

