
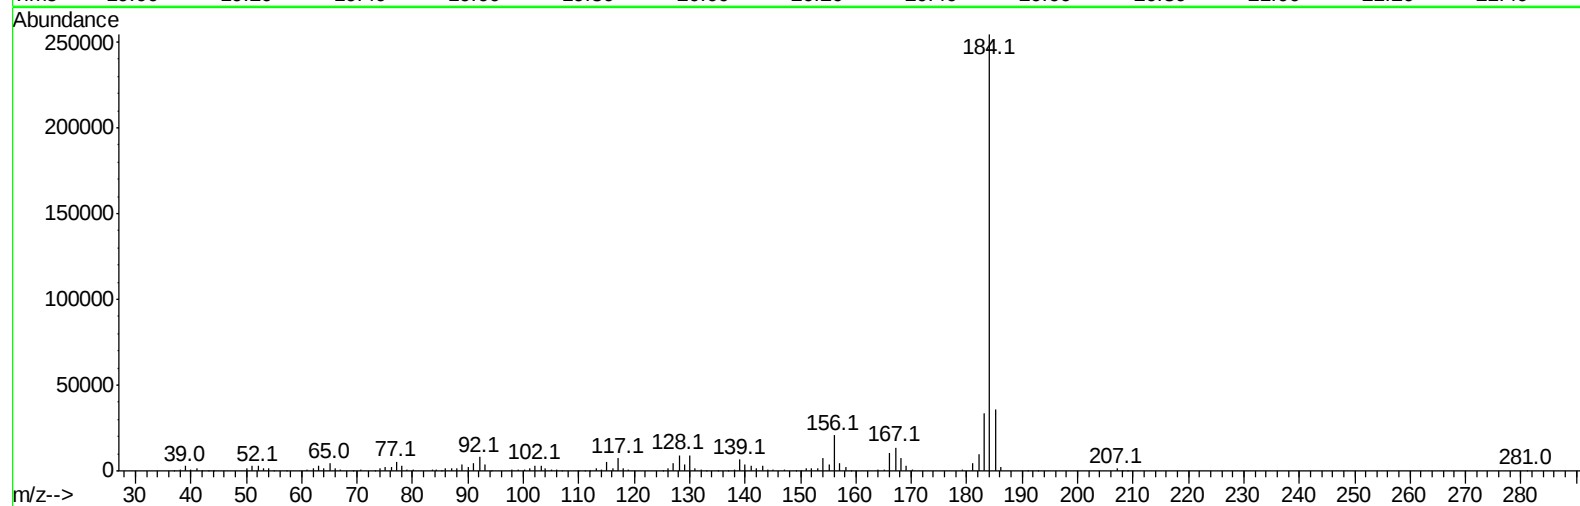


Data Path : U:\HPCHEM1\BNA G\DATA\BG013118\
Data File : BG032460.D
Acq On : 31 Jan 2018 11:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 05:04:58 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

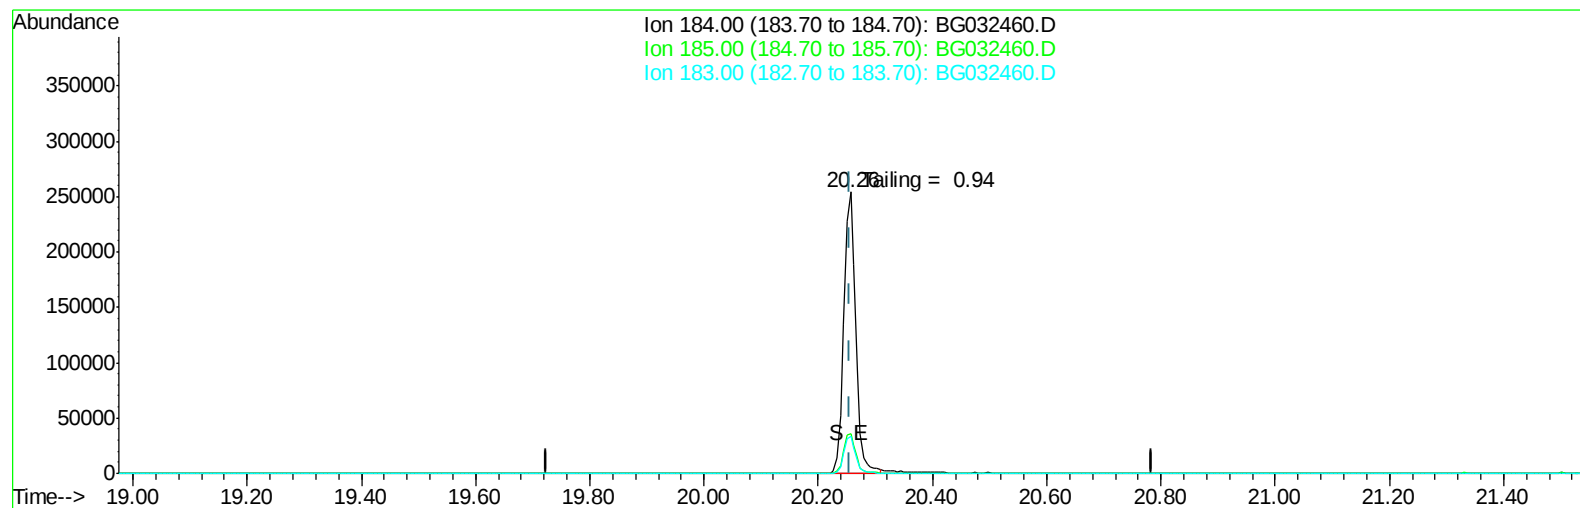

TIC: BG032460.D

(76) Benzidine



20.256min (+0.001) 0.00ng

response 373550

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.20
183.00	13.30	13.31
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG013118\
Data File : BG032460.D
Acq On : 31 Jan 2018 11:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 05:04:58 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

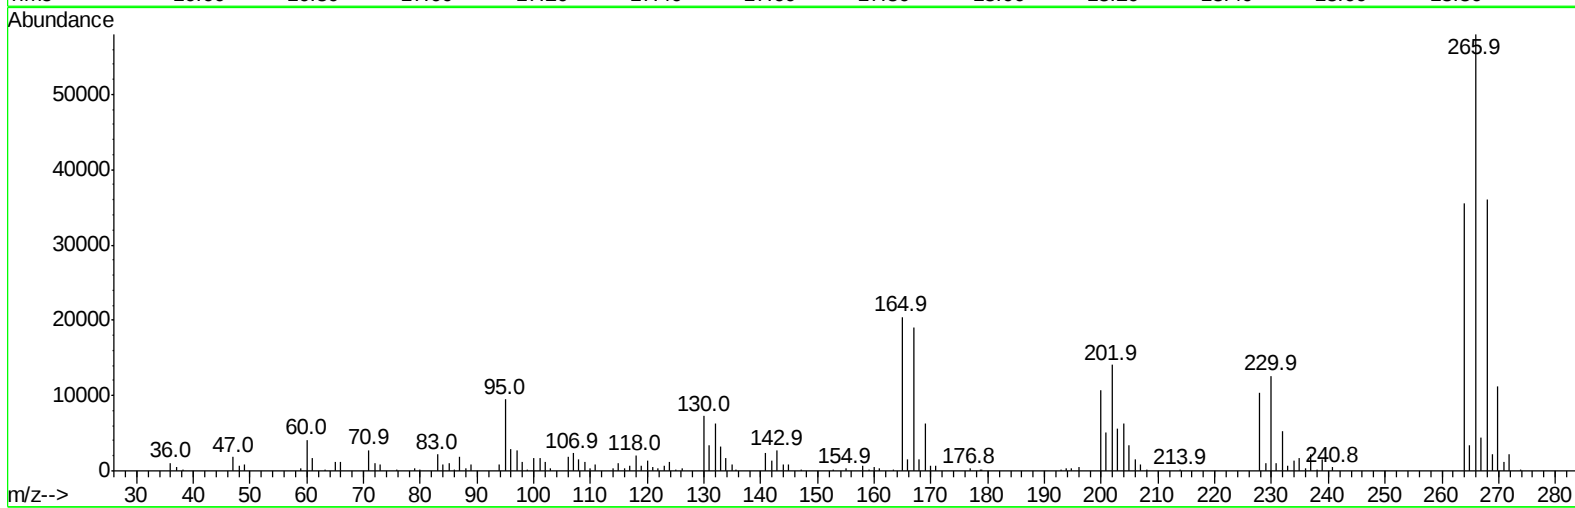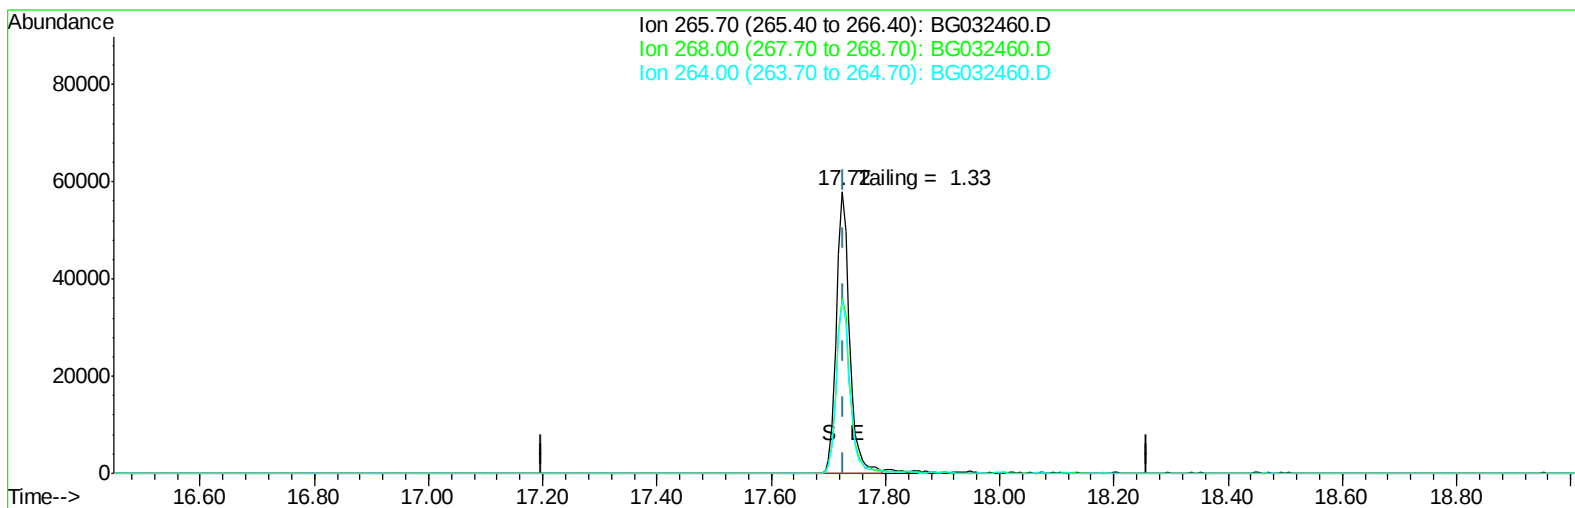

TIC: BG032460.D

(69) Pentachlorophenol (C)

17.724min (-0.005) 35865.97ng

response 92458

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.22
264.00	62.00	61.24
0.00	0.00	0.00