
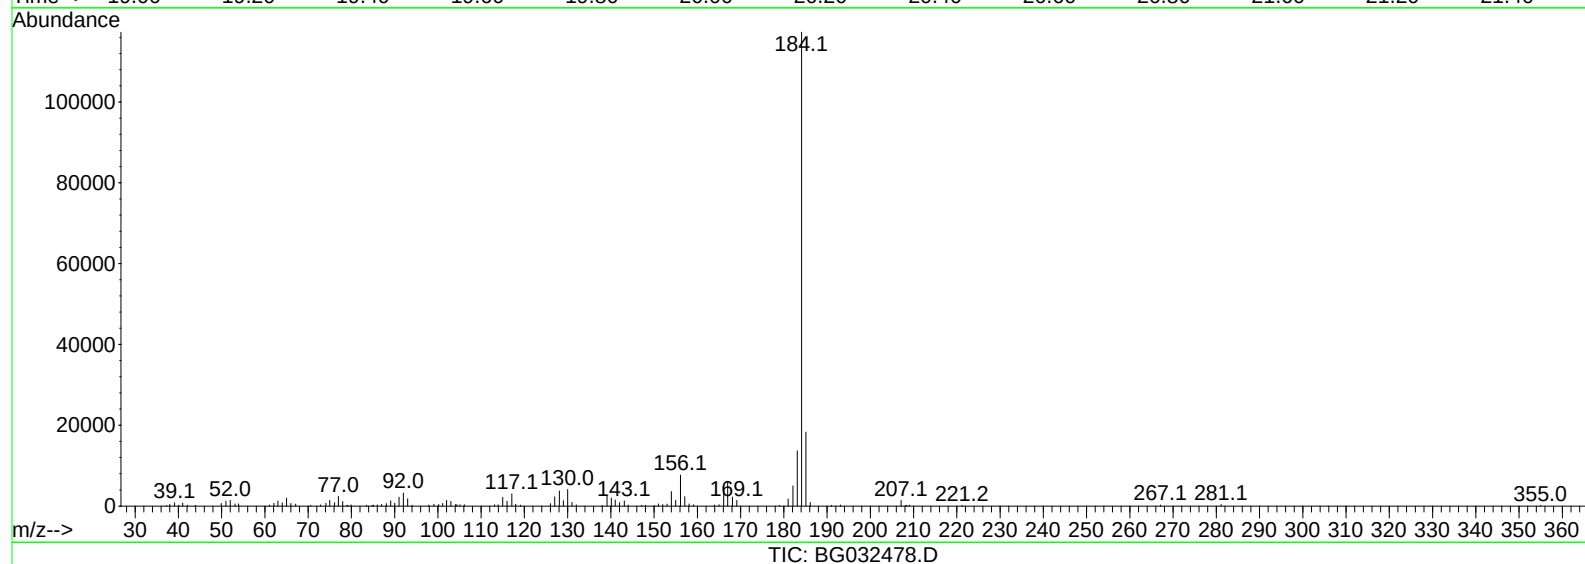


Data Path : U:\HPCHEM1\BNA G\DATA\BG013118\
Data File : BG032478.D
Acq On : 1 Feb 2018 00:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 05:06:30 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

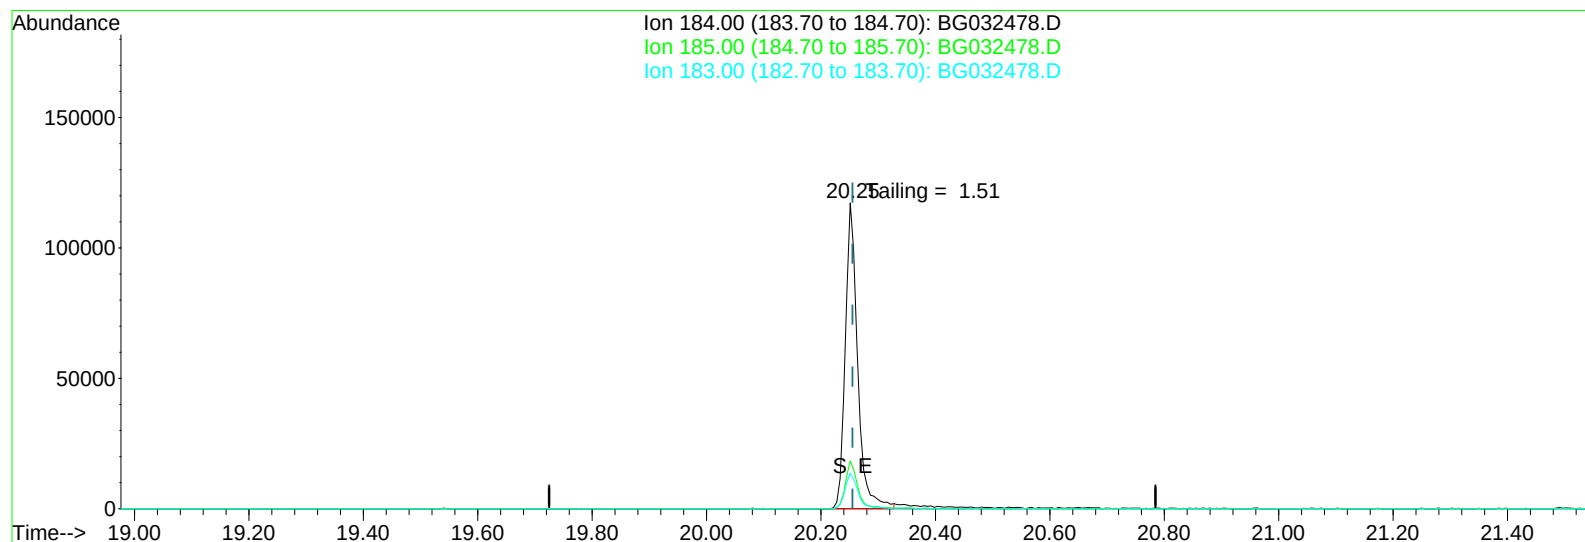

(76) Benzidine



20.251min (-0.004) 160192.69ng

response 179296

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.62
183.00	13.30	11.66
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG013118\
Data File : BG032478.D
Acq On : 1 Feb 2018 00:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 05:06:30 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

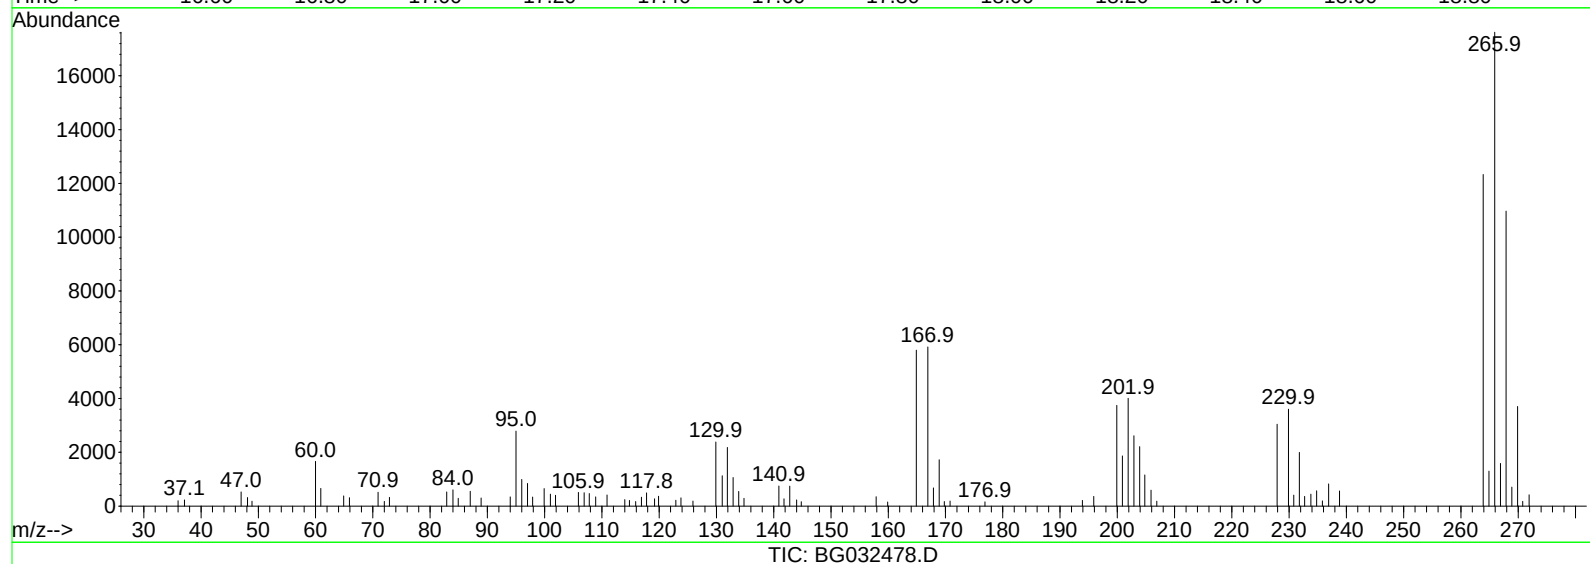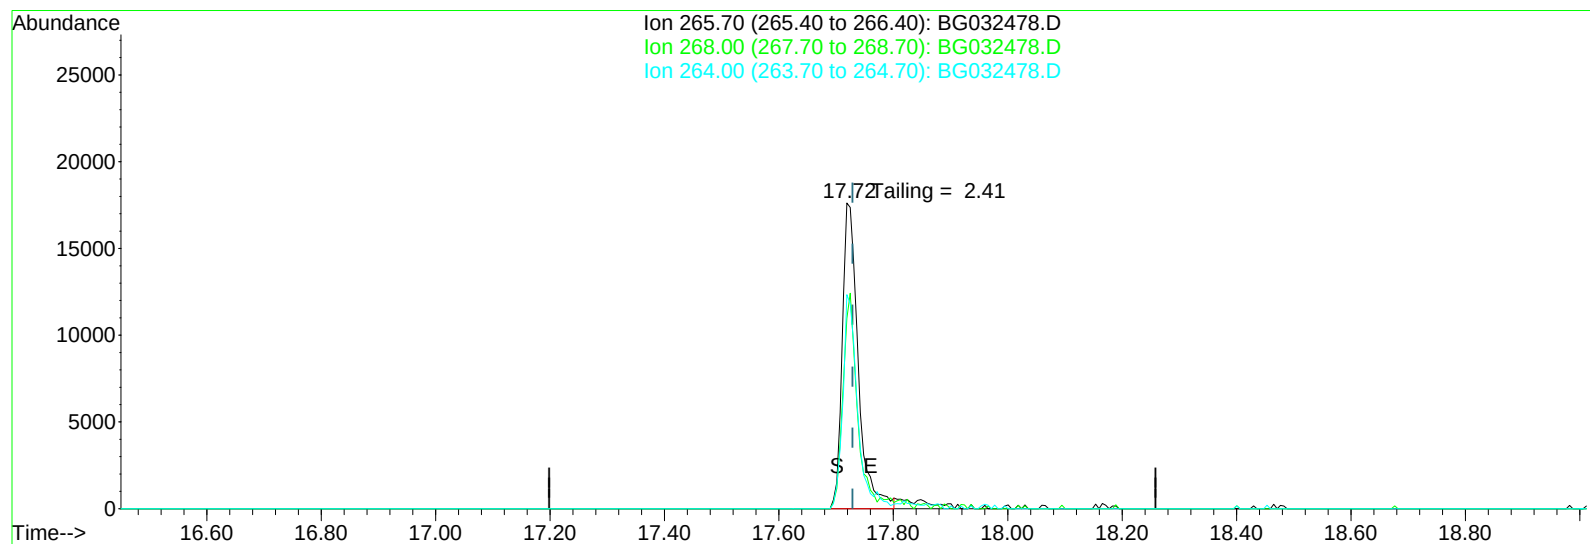

(69) Pentachlorophenol (C)

17.719min (-0.010) 50987.35ng

response 34038

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.23
264.00	62.00	69.98
0.00	0.00	0.00