

Data Path : Z:\HPCHEM1\BNA G\DATA\BG013118\
Data File : BG032470.D
Acq On : 31 Jan 2018 18:00
Operator : SJ/JU
Sample : PB106216BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106216BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.155	481	488	512	rBV	177014	361078	17.16%	4.227%
2	7.835	767	774	799	rBV	173065	373252	17.74%	4.369%
3	8.229	833	841	855	rBV	205995	412565	19.61%	4.830%
4	8.711	917	923	935	rBV2	80483	156584	7.44%	1.833%
5	9.046	972	980	995	rBV	272830	538943	25.61%	6.309%
6	9.909	1119	1127	1140	rBV	168254	348946	16.58%	4.085%
7	11.590	1406	1413	1424	rBV	107682	212579	10.10%	2.489%
8	13.969	1811	1818	1834	rBV	666248	1152127	54.76%	13.487%
9	15.344	2044	2052	2066	rBV2	189812	339614	16.14%	3.976%
10	16.819	2297	2303	2316	rBV	413132	687385	32.67%	8.047%
11	18.076	2511	2517	2529	rVB2	295868	483991	23.00%	5.666%
12	20.615	2943	2949	2959	rBV	1581976	2104025	100.00%	24.630%
13	22.407	3245	3254	3263	rBV2	362146	672459	31.96%	7.872%
14	26.085	3868	3880	3894	rVB2	214076	698852	33.22%	8.181%


Sum of corrected areas: 8542400

Data Path : Z:\HPCHEM1\BNA G\DATA\BG013118\
Data File : BG032470.D
Acq On : 31 Jan 2018 18:00
Operator : SJ/JU
Sample : PB106216BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106216BL

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

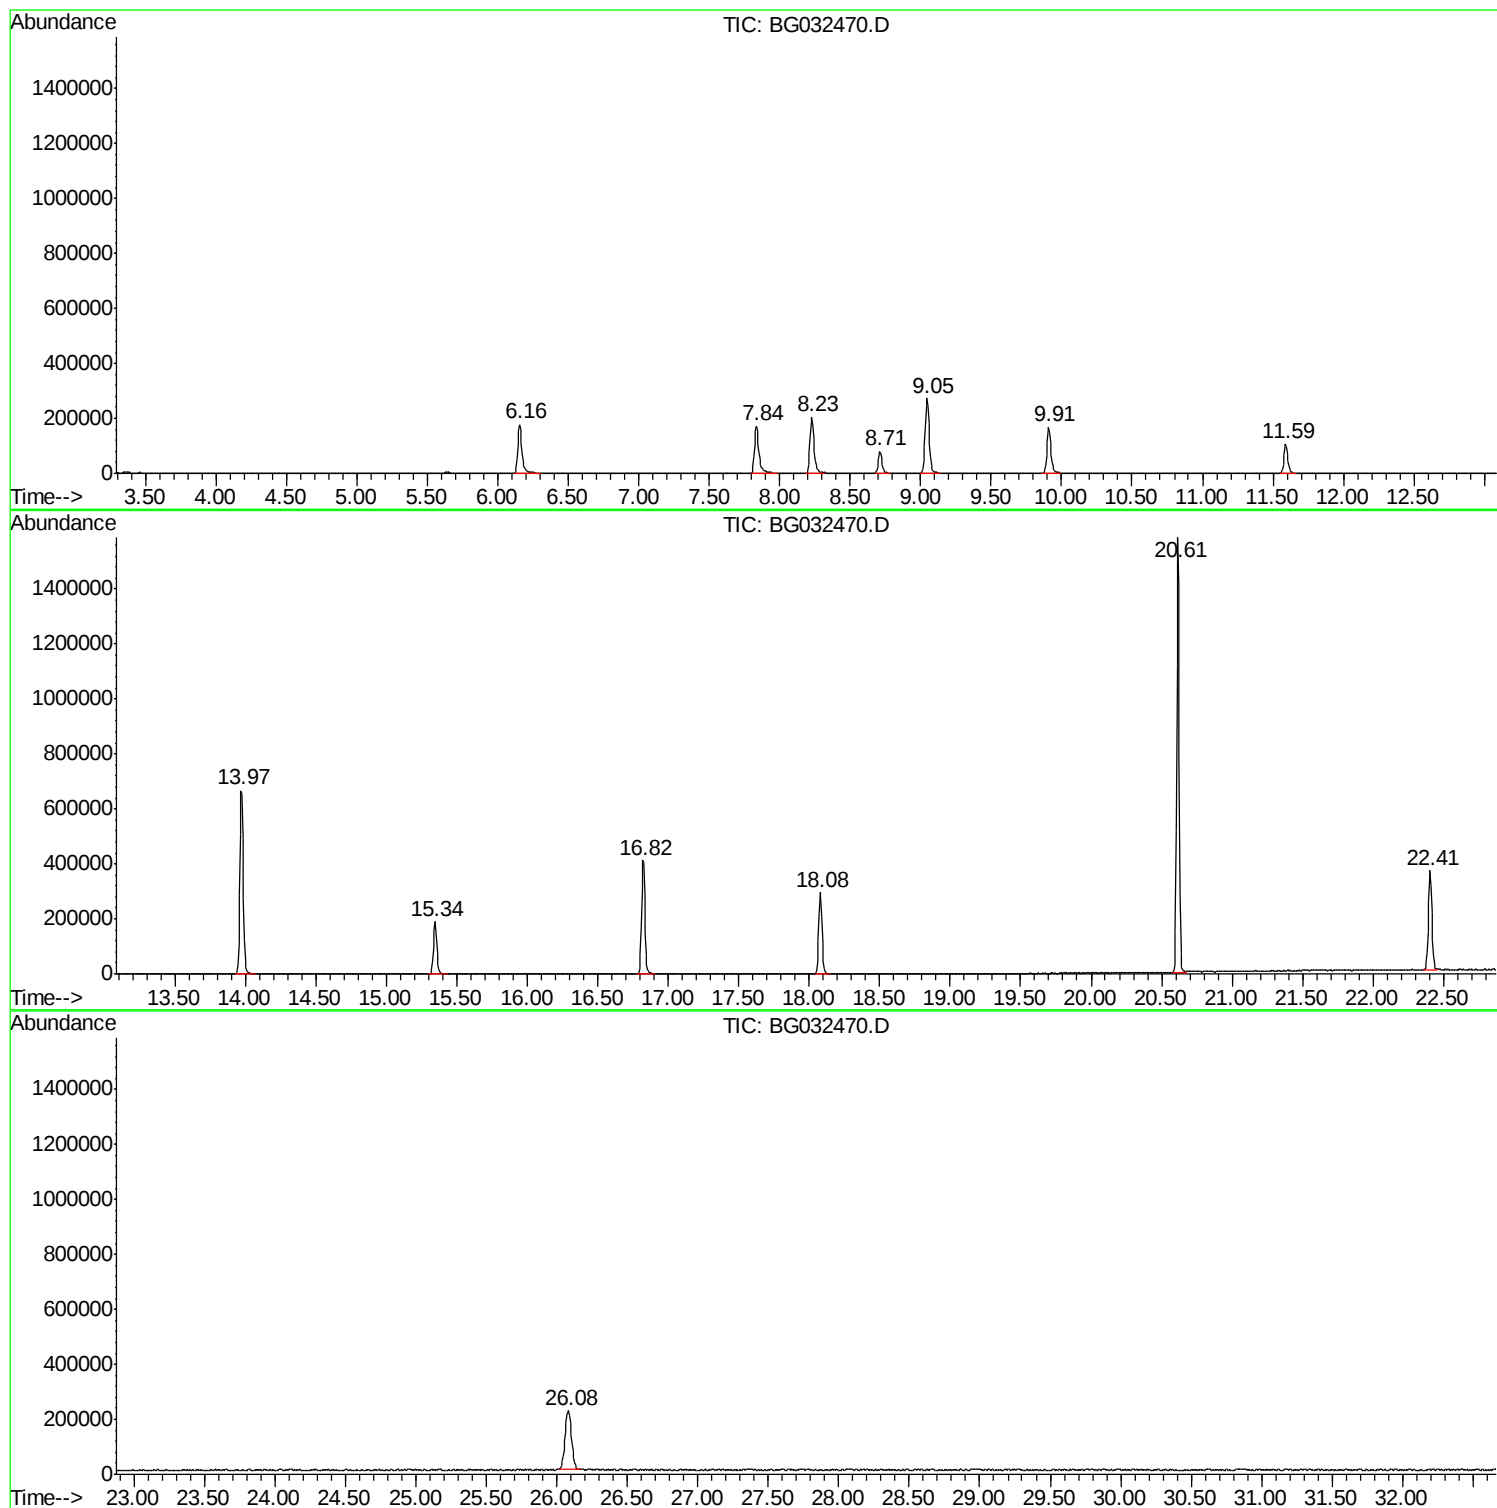

Data Path : Z:\HPCHEM1\BNA G\DATA\BG013118\
Data File : BG032470.D
Acq On : 31 Jan 2018 18:00
Operator : SJ/JU
Sample : PB106216BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106216BL










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown8.23 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.23	52.70 ng	412565	1,4-Dichlorobenzene-d4	8.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	27
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	12

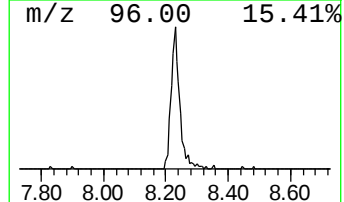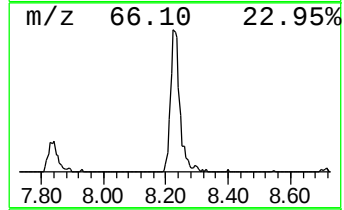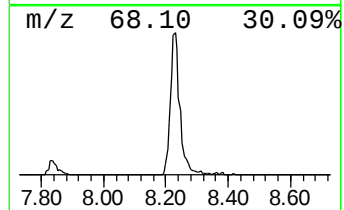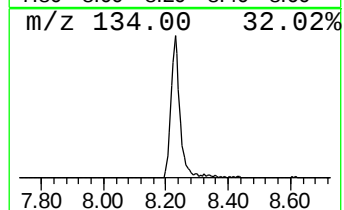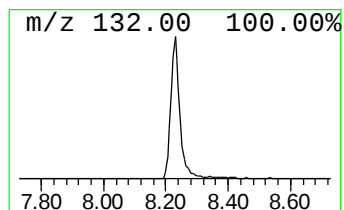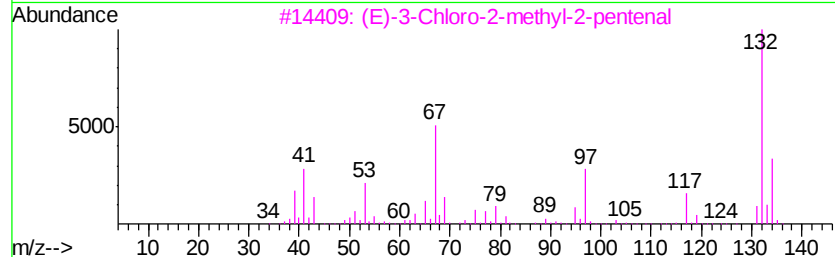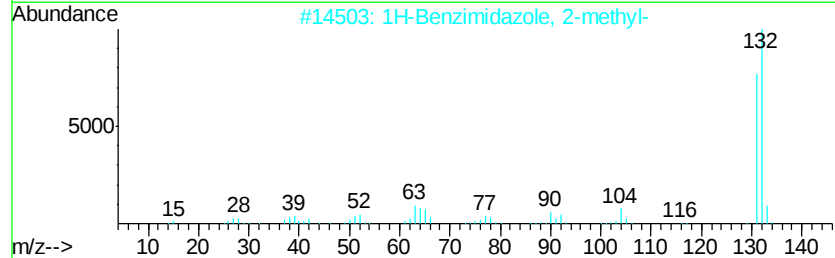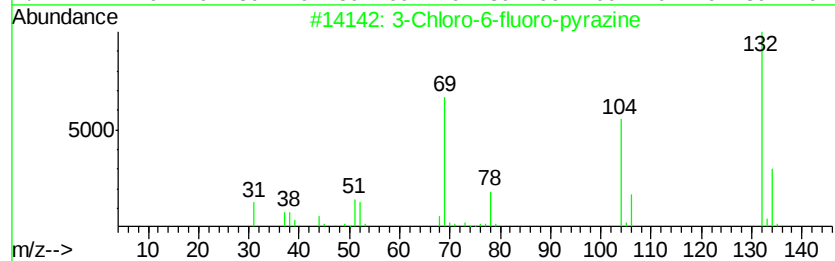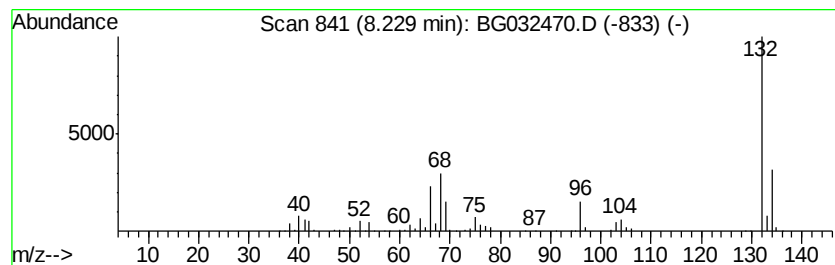

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG013118\
Data File : BG032470.D
Acq On : 31 Jan 2018 18:00
Operator : SJ/JU
Sample : PB106216BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106216BL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.23	8.23	52.7	ng	412565	1	8.71	156584	20.0