


Data Path : Z:\HPCHEM1\BNA G\Data\BG013118\
 Data File : BG032460.D
 Acq On : 31 Jan 2018 11:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 29 15:32:55 2018

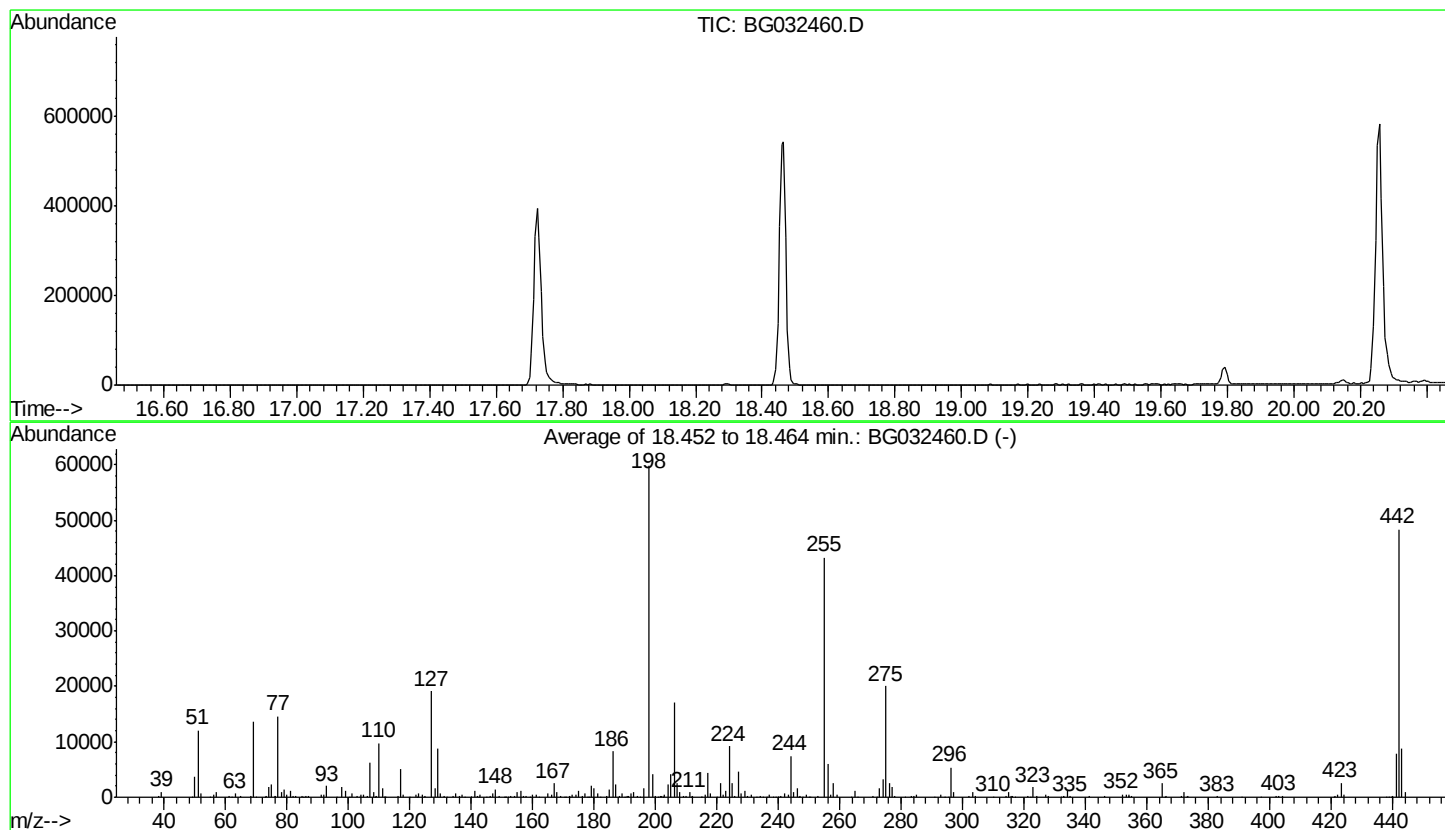

AutoFind: Scans 2581, 2582, 2583; Background Corrected with Scan 2575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.2	12112	PASS
68	69	0.00	2	1.7	231	PASS
69	198	0.00	100	22.7	13566	PASS
70	69	0.00	2	0.5	69	PASS
127	198	10	80	32.0	19155	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59834	PASS
199	198	5	9	6.9	4154	PASS
275	198	10	60	33.6	20094	PASS
365	198	1	100	4.2	2489	PASS
441	442	0.01	24	16.1	7764	PASS
442	198	50	100	80.8	48370	PASS
443	442	15	24	18.3	8842	PASS