


Data Path : Z:\HPCHEM1\BNA G\Data\BG013118\
 Data File : BG032478.D
 Acq On : 1 Feb 2018 00:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 29 15:32:55 2018

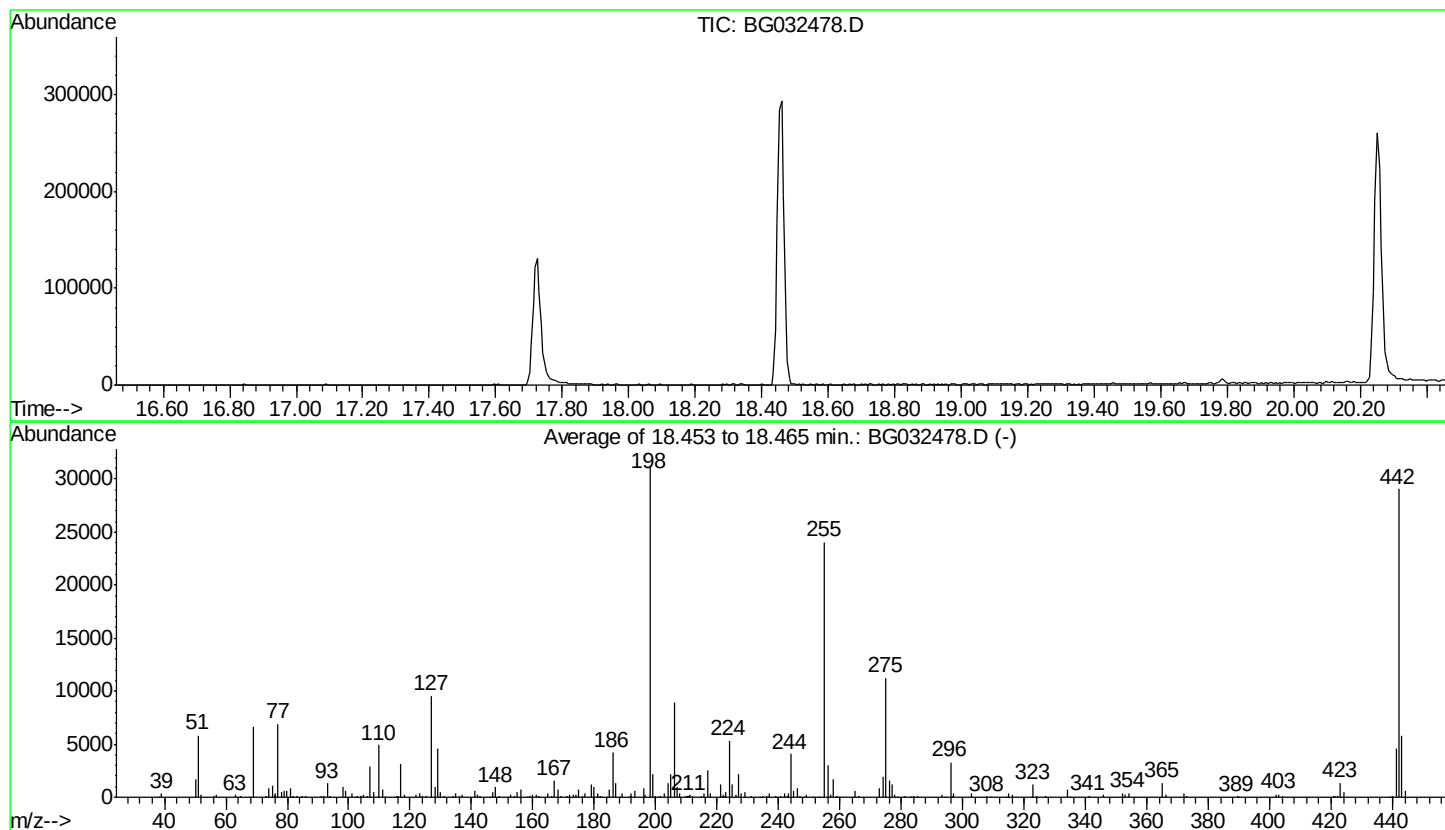

AutoFind: Scans 2581, 2582, 2583; Background Corrected with Scan 2574

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.7	5834	PASS
68	69	0.00	2	0.9	58	PASS
69	198	0.00	100	21.3	6675	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	30.6	9564	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31269	PASS
199	198	5	9	7.0	2187	PASS
275	198	10	60	36.0	11242	PASS
365	198	1	100	4.4	1391	PASS
441	442	0.01	24	15.9	4607	PASS
442	198	50	100	92.9	29040	PASS
443	442	15	24	19.8	5751	PASS