


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG013120\
 Data File : BG044251.D
 Acq On : 31 Jan 2020 9:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 30 16:05:09 2020

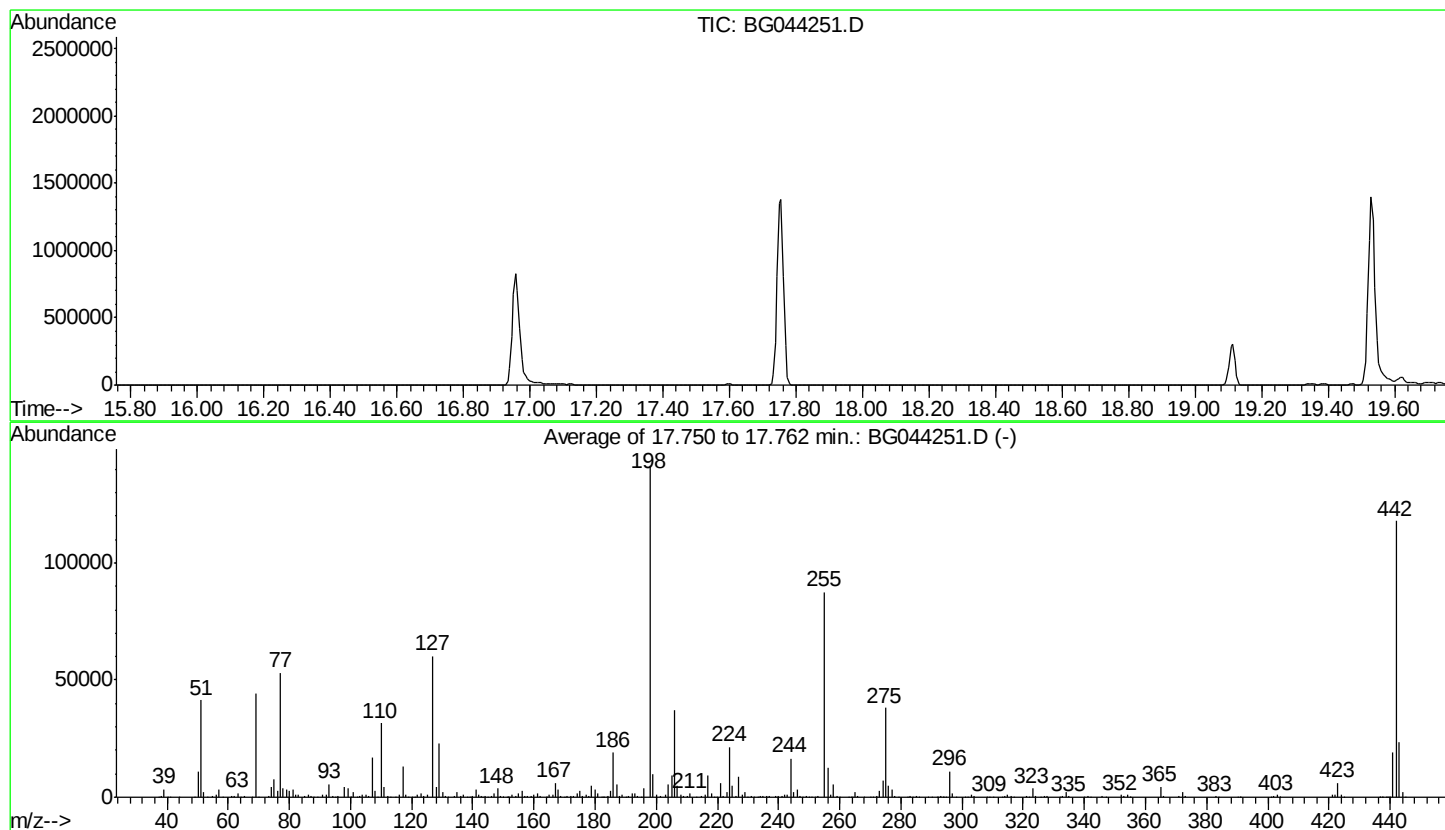

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	41258	PASS
68	69	0.00	2	0.5	207	PASS
69	198	0.00	100	31.4	44432	PASS
70	69	0.00	2	0.6	257	PASS
127	198	10	80	42.5	60176	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	141480	PASS
199	198	5	9	6.8	9680	PASS
275	198	10	60	27.0	38144	PASS
365	198	1	100	3.2	4529	PASS
441	198	0.01	100	13.7	19400	PASS
442	198	50	100	83.2	117778	PASS
443	442	15	24	19.9	23408	PASS