


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013122\
 Data File : BG052213.D
 Acq On : 31 Jan 2022 12:55
 Operator : CG/JU
 Sample : DFTPP460
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP460

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION
 Last Update : Mon Jan 31 18:07:10 2022

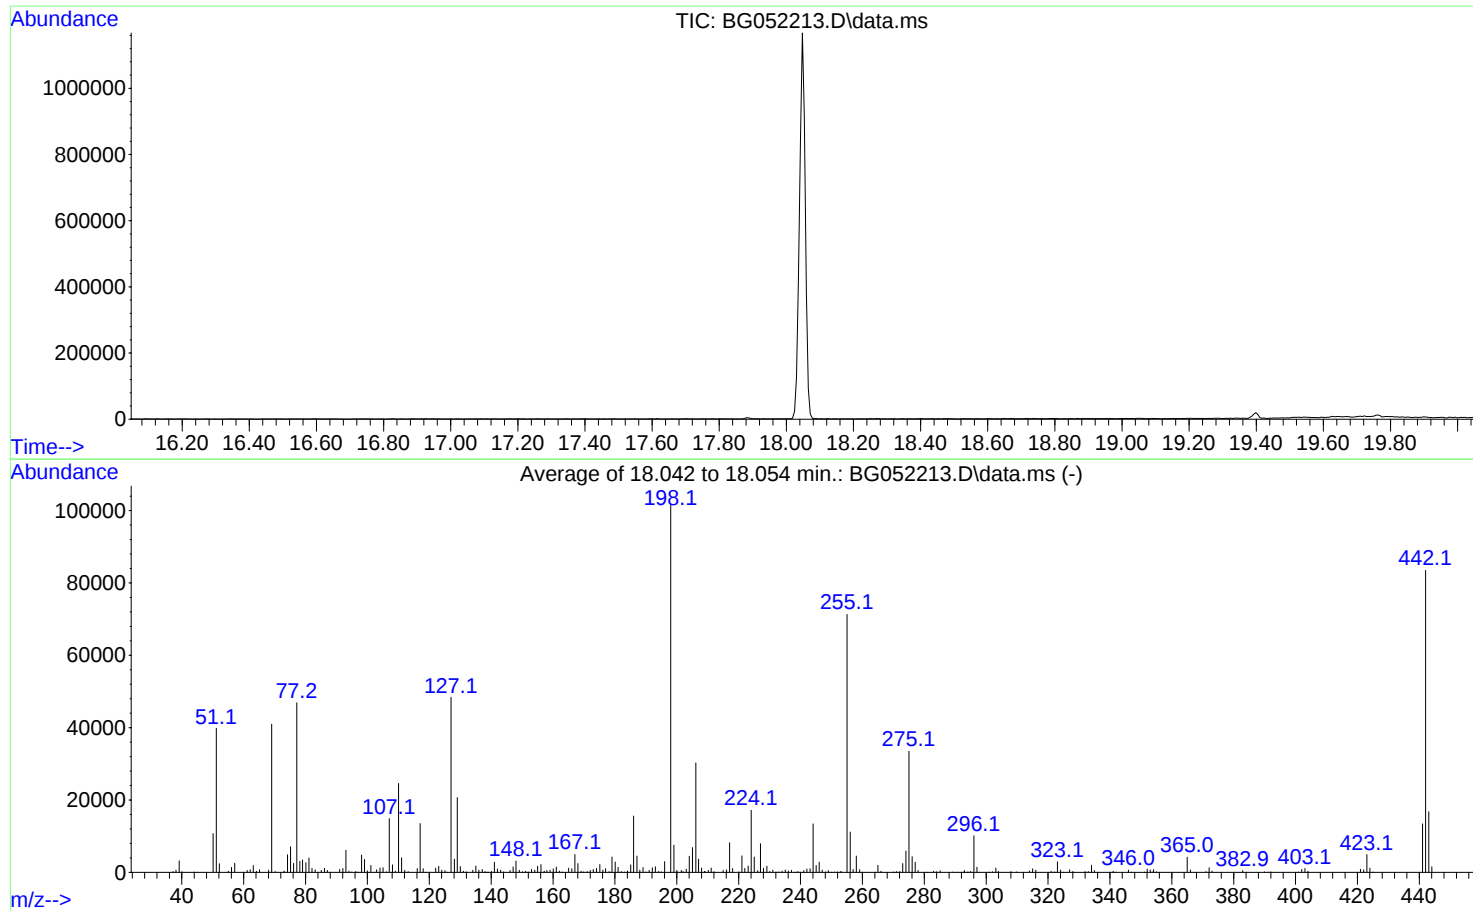

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	39800	PASS
68	69	0.00	2	1.5	625	PASS
69	198	0.00	100	40.3	40941	PASS
70	69	0.00	2	0.5	207	PASS
127	198	10	80	47.6	48376	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101685	PASS
199	198	5	9	7.4	7534	PASS
275	198	10	60	32.9	33469	PASS
365	198	1	100	4.1	4214	PASS
441	198	0.01	100	13.2	13412	PASS
442	198	50	100	82.1	83483	PASS
443	442	15	24	20.1	16775	PASS

Scan 2471 (18.007 min): BG052213.D\data.ms
DFTPP460

m/z	Abundance
40.05	181.0
41.15	237.0
44.05	683.0
206.95	420.0

Instrument :
BNA_G
ClientSampleId :
DFTPP460

m/z	Abundance
37.15	201.0
38.15	594.0
39.15	3022.0
40.15	183.0
41.15	162.0
44.15	839.0
45.15	157.0
50.15	9546.0
51.15	40536.0
52.15	2385.0
55.05	331.0
56.15	1605.0
57.15	2423.0
61.15	537.0
62.15	909.0
63.05	1754.0
64.15	262.0
65.05	589.0
68.05	856.0
69.05	42160.0
70.25	311.0
73.05	435.0
74.15	5064.0
75.15	6515.0
76.15	2440.0
77.15	46336.0
78.15	2751.0
79.05	3246.0
80.05	2563.0
81.15	4074.0
82.05	1034.0
83.15	664.0
85.15	642.0
86.05	871.0
87.05	614.0
91.05	817.0
92.05	935.0
93.05	5686.0
94.05	399.0
96.25	216.0
96.55	200.0
98.15	4265.0
99.05	3603.0
99.95	259.0
101.15	1765.0
103.05	698.0
104.05	1249.0
105.05	1027.0
106.15	486.0
107.05	13314.0
108.05	2231.0
110.05	23544.0
111.05	3571.0
112.05	562.0
113.25	233.0
116.05	982.0
117.05	12219.0
118.05	893.0
122.05	1068.0
123.05	1528.0
124.05	517.0
125.05	381.0
127.05	45528.0
128.15	3686.0
129.05	18328.0
130.05	1595.0
131.05	285.0
134.05	616.0
135.05	1501.0
136.05	591.0
137.05	792.0
138.25	157.0
138.85	164.0
140.15	232.0
141.05	2673.0
142.05	954.0
143.05	638.0
144.05	188.0
146.15	543.0
147.05	1542.0
148.05	2817.0
149.15	531.0
150.15	188.0
151.05	405.0
152.15	156.0
153.05	646.0
154.05	429.0
154.95	1497.0
156.05	1688.0
157.05	315.0
157.95	358.0
159.05	645.0

Instrument :
BNA_G
ClientSampleId :
DFTPP460

160.05	1073.0
161.05	1333.0
162.05	416.0
165.15	1025.0
166.05	1071.0
167.05	4592.0
168.05	2522.0
169.05	389.0
169.95	224.0
171.05	224.0
172.05	577.0
172.95	554.0
174.05	840.0
175.15	2222.0
176.15	561.0
176.95	741.0
178.15	288.0
179.05	4178.0
180.05	2440.0
181.05	1231.0
182.05	244.0
184.15	416.0
185.15	1673.0
186.05	14370.0
187.15	4347.0
188.05	714.0
189.05	1072.0
191.05	592.0
192.15	1204.0
193.05	1583.0
194.15	224.0
195.05	215.0
196.05	2514.0
198.05	88792.0
199.05	6328.0
199.85	584.0
201.45	659.0
203.05	727.0
204.05	3793.0
205.05	6455.0
206.15	25640.0
207.15	3816.0
208.05	1000.0
208.95	360.0
210.15	345.0
211.05	1086.0
215.05	427.0
216.15	491.0
217.05	7774.0
218.05	1109.0
220.15	231.0
221.05	3998.0
222.05	793.0
223.05	1602.0
224.05	13559.0
225.05	4069.0
226.25	409.0
227.05	6361.0
228.05	1077.0
229.15	1501.0
230.05	207.0
231.05	488.0
234.05	352.0
235.05	718.0
236.05	351.0
237.05	515.0
238.25	205.0
238.95	202.0
240.95	442.0
242.05	845.0
243.05	684.0
244.05	11331.0
245.05	1187.0
246.05	2503.0
247.05	474.0
248.95	386.0
252.85	356.0
255.05	56752.0
256.05	9012.0
257.05	574.0
258.05	3578.0
259.15	745.0
260.05	191.0
265.05	1656.0
265.95	262.0
270.25	177.0
271.05	248.0
272.05	208.0
272.95	2395.0
274.05	4597.0
275.05	27080.0
276.05	3572.0
277.05	2346.0
277.95	268.0
281.05	165.0
283.05	166.0

Instrument :
BNA_G
ClientSampleId :
DFTPP460

283.95	180.0
285.05	422.0
292.85	596.0
295.05	253.0
296.05	7504.0
297.05	1101.0
303.15	970.0
303.95	231.0
308.05	179.0
309.95	196.0
314.15	187.0
315.05	866.0
316.05	426.0
320.95	158.0
323.05	2297.0
324.05	438.0
325.05	167.0
326.95	654.0
327.95	174.0
332.05	160.0
334.05	1621.0
335.05	520.0
340.95	285.0
346.05	507.0
352.05	706.0
352.95	312.0
353.95	588.0
364.95	2891.0
365.95	433.0
372.05	1027.0
373.05	325.0
382.85	223.0
384.15	168.0
391.95	220.0
401.95	457.0
403.05	773.0
403.95	206.0
421.05	446.0
421.95	489.0
423.05	3116.0
424.05	884.0
441.05	9732.0
442.05	56568.0
443.05	12133.0
444.05	845.0

Instrument :
BNA_G
ClientSampleId :
DFTPP460

m/z	Abundance
37.15	316.0
38.15	866.0
39.15	4105.0
40.05	378.0
41.15	266.0
44.05	819.0
50.15	13577.0
51.15	46416.0
52.15	2860.0
55.05	430.0
56.05	1398.0
57.15	3151.0
61.15	682.0
62.15	742.0
63.15	2165.0
64.15	337.0
65.15	766.0
68.05	1019.0
69.05	49520.0
70.15	310.0
73.05	643.0
74.15	5375.0
75.15	8704.0
76.15	3176.0
77.15	57208.0
78.15	3974.0
79.05	4006.0
80.05	3351.0
81.05	4707.0
82.05	1369.0
83.05	1111.0
85.05	748.0
86.15	1461.0
87.05	592.0
91.05	993.0
92.05	1332.0
93.05	7543.0
94.15	421.0
94.95	214.0
96.15	209.0
97.05	168.0
98.15	6147.0
99.05	4647.0
100.05	554.0
101.05	2617.0
102.15	181.0
103.05	840.0
104.05	1548.0
105.05	1671.0
107.05	17632.0
108.15	2664.0
109.05	578.0
110.05	29336.0
111.05	5141.0
112.05	553.0
113.15	186.0
116.15	1473.0
117.05	17168.0
118.05	1217.0
118.95	161.0
120.25	158.0
122.05	1306.0
123.05	2138.0
124.05	847.0
125.05	708.0
125.75	198.0
127.05	58776.0
128.05	4550.0
129.05	25656.0
130.05	1794.0
131.05	391.0
131.95	234.0
134.05	775.0
135.05	2158.0
136.05	746.0
137.15	861.0
137.95	500.0
139.25	188.0
140.05	405.0
141.05	3263.0
142.05	1018.0
143.05	798.0
146.15	604.0
147.15	1685.0
148.05	3704.0
149.05	751.0
150.15	342.0
151.15	341.0
151.85	193.0
153.05	1040.0
154.15	895.0
155.05	1903.0

Instrument :
BNA_G
ClientSampleId :
DFTPP460

156.05	2673.0
157.25	465.0
158.05	783.0
159.05	768.0
160.05	1024.0
161.05	1916.0
161.95	351.0
162.85	215.0
165.05	1614.0
166.15	1185.0
167.05	5414.0
168.05	2776.0
168.95	314.0
171.15	171.0
171.95	434.0
173.05	1109.0
174.05	1438.0
175.05	2691.0
176.15	812.0
177.05	1423.0
178.05	354.0
179.05	5041.0
180.05	3951.0
180.95	1600.0
182.05	262.0
183.95	522.0
185.15	2492.0
186.05	17592.0
187.05	5147.0
187.95	682.0
189.15	1546.0
190.05	275.0
191.05	481.0
192.05	1388.0
193.05	1593.0
194.15	376.0
194.95	192.0
196.05	3187.0
198.05	123352.0
199.05	9535.0
200.05	948.0
201.45	659.0
201.95	433.0
203.05	1063.0
204.05	5645.0
205.05	7894.0
206.15	36872.0
207.05	5077.0
208.05	1294.0
208.95	451.0
210.25	672.0
211.05	1410.0
212.05	364.0
215.05	572.0
216.05	902.0
217.05	9275.0
218.05	1026.0
219.95	212.0
221.05	4929.0
222.05	1347.0
223.05	2112.0
224.05	21248.0
225.05	4502.0
226.15	557.0
227.05	9965.0
228.05	1284.0
229.05	2014.0
230.05	376.0
231.05	957.0
232.95	182.0
234.05	442.0
235.05	765.0
236.05	518.0
237.05	716.0
239.15	544.0
241.05	579.0
242.05	1244.0
243.15	1256.0
244.05	15902.0
245.05	2438.0
246.05	3316.0
246.95	600.0
248.25	161.0
248.95	583.0
251.05	257.0
251.95	210.0
253.15	434.0
255.05	84880.0
256.05	13789.0
256.95	1140.0
258.05	5095.0
259.05	897.0
264.15	170.0
265.05	2343.0
266.05	468.0
271.05	310.0

Instrument :
BNA_G
ClientSampleId :
DFTPP460

272.15	223.0
272.95	2499.0
274.05	6843.0
275.05	40512.0
276.05	5103.0
277.05	3375.0
278.05	607.0
283.05	459.0
283.85	395.0
285.05	560.0
289.15	258.0
290.15	156.0
290.95	167.0
291.85	186.0
293.05	715.0
293.95	208.0
294.95	226.0
296.05	12143.0
296.95	1824.0
297.95	200.0
302.05	239.0
303.05	1503.0
303.95	437.0
307.95	240.0
309.85	239.0
313.95	515.0
315.05	920.0
316.05	862.0
321.05	504.0
322.15	303.0
323.05	3553.0
324.05	745.0
326.95	858.0
328.15	283.0
332.05	294.0
333.05	291.0
334.05	2209.0
334.95	524.0
340.05	152.0
341.15	347.0
345.95	693.0
351.15	225.0
352.05	1017.0
353.05	974.0
354.15	1149.0
355.05	285.0
365.05	4905.0
366.05	884.0
371.05	345.0
372.05	1340.0
372.95	300.0
382.95	585.0
389.95	199.0
400.95	218.0
401.95	793.0
403.05	1176.0
404.05	457.0
421.05	913.0
421.95	775.0
423.05	5474.0
424.05	1076.0
425.05	261.0
441.05	14796.0
442.05	94496.0
443.05	19200.0
444.05	1902.0

Instrument :
BNA_G
ClientSampleId :
DFTPP460

m/z	Abundance
37.25	209.0
38.15	359.0
39.15	2494.0
40.15	518.0
44.05	602.0
50.15	8930.0
51.15	32448.0
52.15	1967.0
55.05	202.0
56.05	1120.0
57.05	1991.0
61.05	347.0
62.15	427.0
63.05	1641.0
64.15	215.0
65.05	715.0
69.05	31144.0
73.25	398.0
74.15	4184.0
75.15	6090.0
76.15	1894.0
77.15	37120.0
78.15	2495.0
79.05	3160.0
80.15	2143.0
81.05	3193.0
82.15	890.0
83.05	398.0
85.05	399.0
86.05	992.0
87.05	440.0
88.05	150.0
91.05	601.0
92.05	989.0
93.05	5132.0
93.95	240.0
96.15	316.0
98.05	3924.0
99.15	2507.0
100.05	486.0
101.05	1372.0
102.85	577.0
103.95	798.0
105.05	1105.0
107.05	13589.0
108.05	1393.0
109.05	461.0
110.05	20856.0
111.05	3341.0
112.15	636.0
113.05	196.0
116.05	679.0
117.05	11042.0
118.05	976.0
122.05	1226.0
123.05	1360.0
124.05	551.0
125.05	440.0
127.05	40824.0
128.05	2674.0
129.05	18024.0
130.05	1378.0
131.05	258.0
132.05	198.0
134.05	354.0
135.05	1645.0
136.05	564.0
137.15	702.0
138.05	208.0
140.05	183.0
141.05	2481.0
142.05	773.0
143.15	409.0
144.05	188.0
145.95	440.0
147.05	1315.0
148.05	2948.0
149.05	468.0
151.05	232.0
152.15	165.0
153.05	722.0
154.05	493.0
155.05	1602.0
156.15	2130.0
157.15	427.0
158.05	457.0
159.05	282.0
160.05	883.0
161.05	1137.0
162.15	293.0
163.15	180.0
164.95	836.0

Instrument :
BNA_G
ClientSampleId :
DFTPP460

166.15	815.0
167.05	4912.0
168.05	1939.0
169.15	199.0
169.85	212.0
170.95	241.0
171.95	591.0
172.95	792.0
174.05	1106.0
175.15	1610.0
176.05	545.0
176.95	959.0
179.05	3498.0
180.15	2254.0
181.05	1354.0
182.05	185.0
183.15	222.0
184.05	313.0
185.05	2088.0
186.05	14770.0
187.05	4032.0
188.15	513.0
189.05	1414.0
189.95	160.0
191.05	607.0
192.05	1228.0
193.05	1425.0
194.05	173.0
196.05	3251.0
198.05	92912.0
199.05	6740.0
200.05	639.0
201.55	346.0
202.05	240.0
203.05	850.0
204.05	3939.0
205.05	6256.0
206.15	28264.0
207.15	3450.0
207.95	1301.0
209.15	488.0
210.25	633.0
211.15	1084.0
211.95	211.0
214.95	606.0
216.05	794.0
217.05	7533.0
218.05	1092.0
221.05	4785.0
221.95	1234.0
223.05	1644.0
224.05	16632.0
225.05	4230.0
226.05	444.0
227.05	7445.0
228.05	1071.0
229.05	1698.0
230.05	277.0
231.05	434.0
232.05	223.0
233.05	182.0
234.05	342.0
235.05	502.0
236.05	340.0
237.15	436.0
239.15	191.0
240.05	175.0
241.15	432.0
242.05	676.0
243.15	1080.0
244.05	12985.0
245.05	2066.0
246.05	2704.0
247.05	825.0
248.05	233.0
249.05	552.0
249.95	180.0
251.75	258.0
253.05	421.0
255.05	72328.0
256.05	10707.0
257.05	741.0
258.05	4911.0
259.05	616.0
264.95	1831.0
266.05	193.0
269.95	206.0
270.95	162.0
272.05	200.0
273.05	2484.0
274.05	6267.0
275.05	32816.0
276.05	4365.0
277.05	2641.0
277.95	689.0
282.95	364.0

Instrument :
BNA_G
ClientSampleId :
DFTPP460

284.15	200.0
285.15	389.0
292.95	778.0
294.15	306.0
294.95	349.0
296.05	10742.0
297.05	1315.0
300.95	262.0
302.05	260.0
303.05	1070.0
304.05	172.0
307.95	266.0
313.95	545.0
314.95	1087.0
316.05	589.0
320.95	263.0
322.05	163.0
323.05	2962.0
324.05	727.0
326.95	673.0
327.95	335.0
331.85	186.0
332.95	364.0
334.05	2025.0
335.05	486.0
341.05	457.0
341.95	179.0
346.05	609.0
347.05	249.0
352.05	1042.0
353.05	657.0
354.05	1054.0
355.15	292.0
364.95	4847.0
366.05	717.0
370.95	276.0
372.05	1527.0
373.05	409.0
382.85	656.0
390.05	269.0
391.15	207.0
391.95	172.0
402.05	1129.0
403.05	1260.0
404.05	323.0
420.95	1111.0
422.05	910.0
423.05	6090.0
424.05	1592.0
441.05	15708.0
442.05	99384.0
443.05	18992.0
444.05	1844.0

Instrument :
BNA_G
ClientSampleId :
DFTPP460