
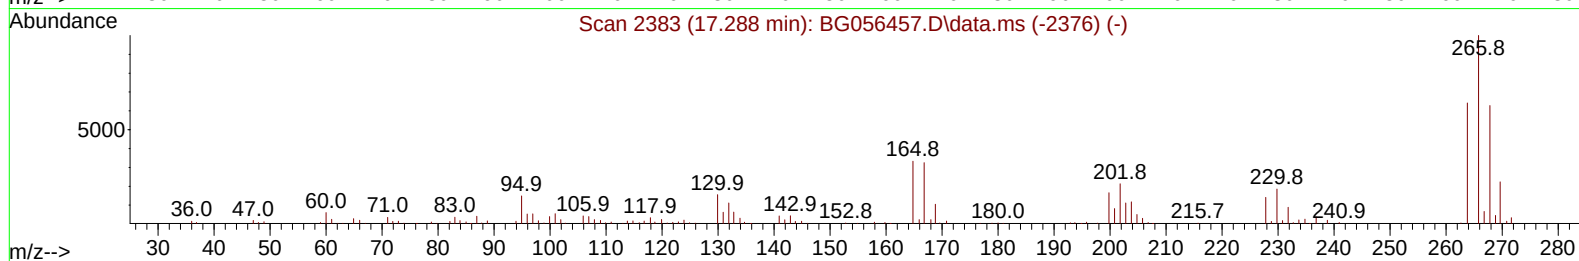
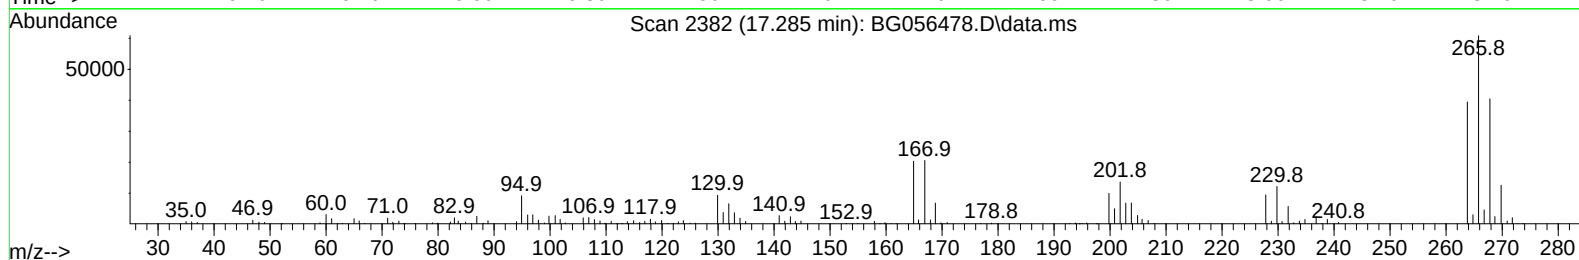


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013123\
Data File : BG056478.D
Acq On : 31 Jan 2023 9:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 03:21:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:15:52 2023
Response via : Initial Calibration

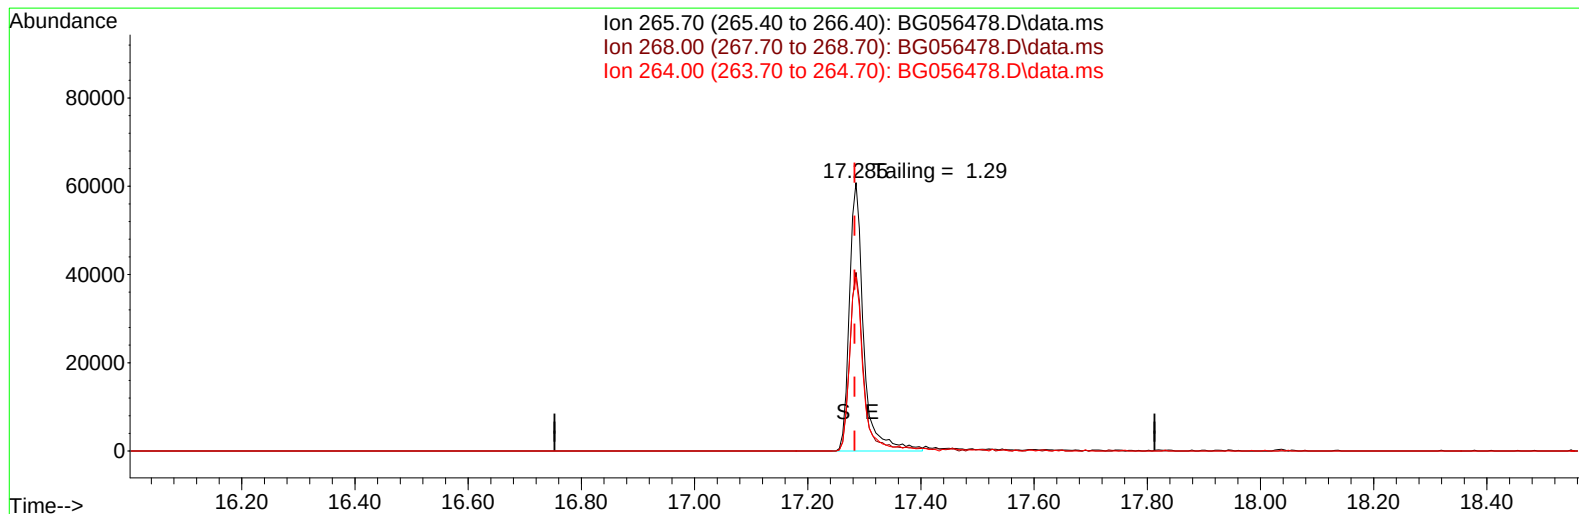

TIC: BG056478.D\data.ms

(70) Pentachlorophenol (C)




17.285min (+ 0.003) 22471.26 ng

response 106723

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	70.60
264.00	64.20	64.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013123\
Data File : BG056478.D
Acq On : 31 Jan 2023 9:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 03:21:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:15:52 2023
Response via : Initial Calibration

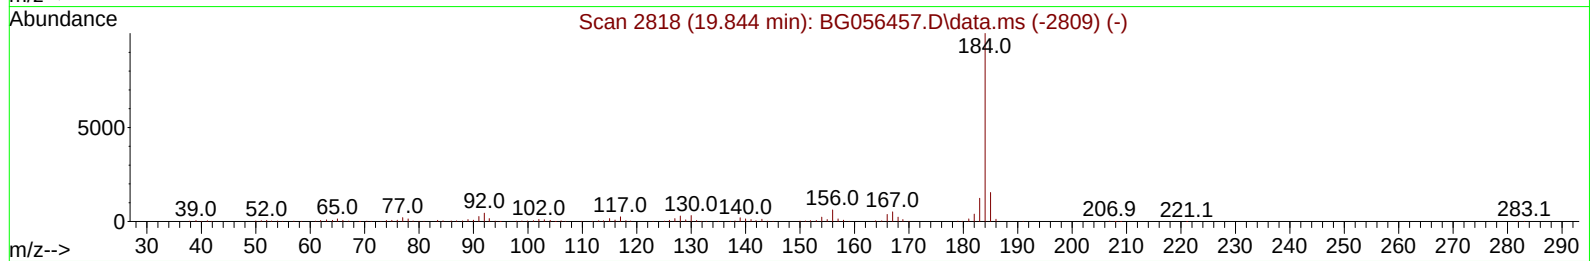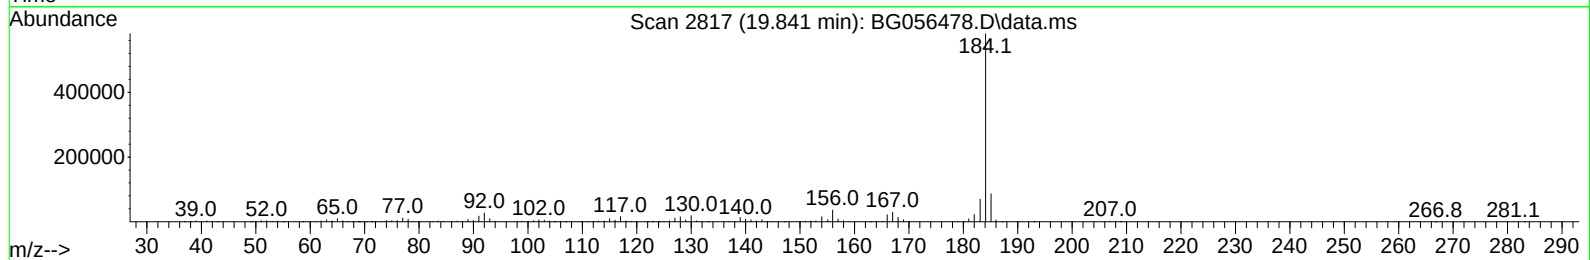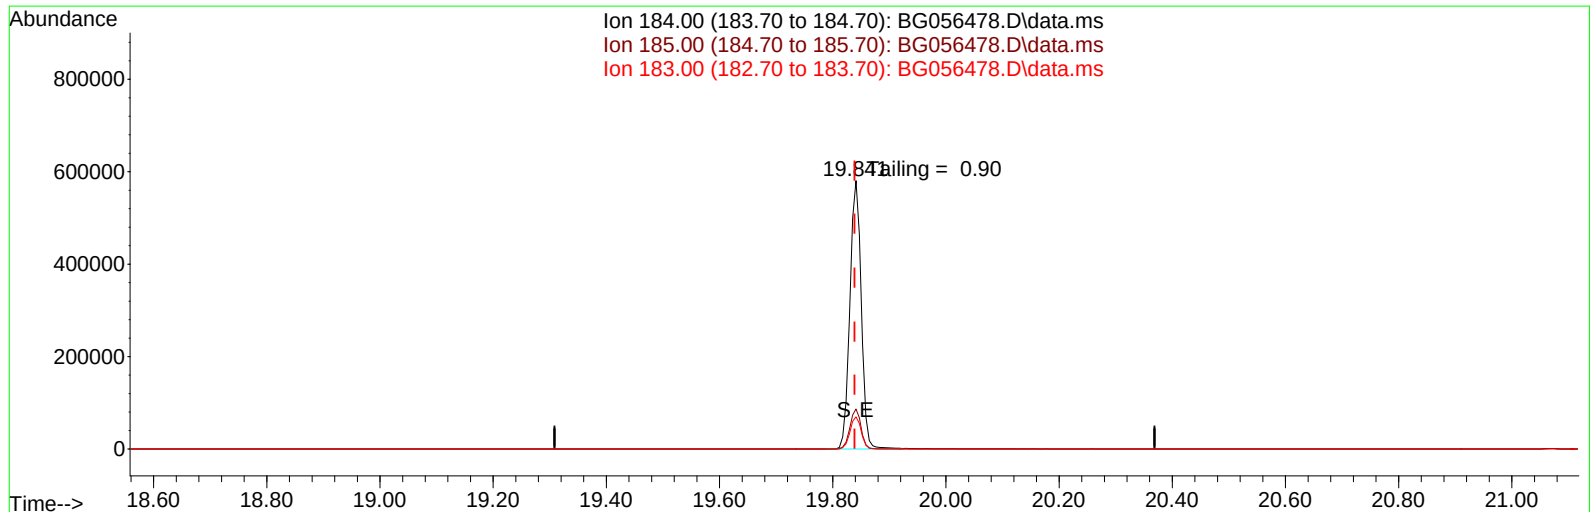

TIC: BG056478.D\data.ms

(77) Benzidine

19.841min (+ 0.003) 142958.10 ng

response 812410

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.90
183.00	12.30	12.02
0.00	0.00	0.00