

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013123\
Data File : BG056491.D
Acq On : 31 Jan 2023 18:56
Operator : CG/JU
Sample : PB150200BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150200BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.307	336	343	352	rBV	104400	158896	4.61%	1.399%
2	5.794	419	426	436	rBV	451480	726615	21.06%	6.396%
3	7.422	694	703	715	rBV	449713	768879	22.28%	6.768%
4	8.274	842	848	855	rBB2	93472	154516	4.48%	1.360%
5	9.449	1041	1048	1058	rBV	259971	466694	13.53%	4.108%
6	11.106	1322	1330	1339	rBV	127097	231216	6.70%	2.035%
7	13.521	1734	1741	1753	rBV	1095535	1688133	48.93%	14.859%
8	14.896	1968	1975	1982	rBV	271702	405984	11.77%	3.573%
9	16.376	2220	2227	2247	rBV	826370	1256046	36.40%	11.056%
10	17.633	2434	2441	2452	rBV	398915	601275	17.43%	5.292%
11	20.213	2873	2880	2886	rBV	2567848	3450252	100.00%	30.369%
12	21.923	3164	3171	3182	rBV2	422913	718200	20.82%	6.322%
13	25.342	3742	3753	3766	rVB2	241480	734412	21.29%	6.464%




Sum of corrected areas: 11361118

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013123\
Data File : BG056491.D
Acq On : 31 Jan 2023 18:56
Operator : CG/JU
Sample : PB150200BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150200BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

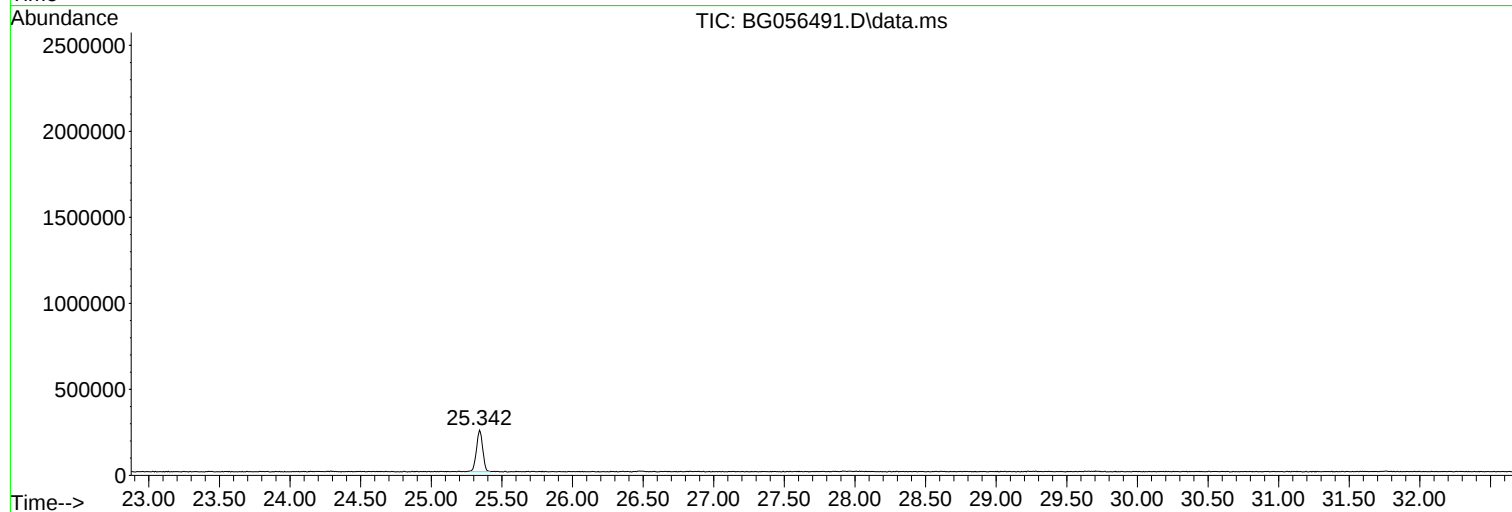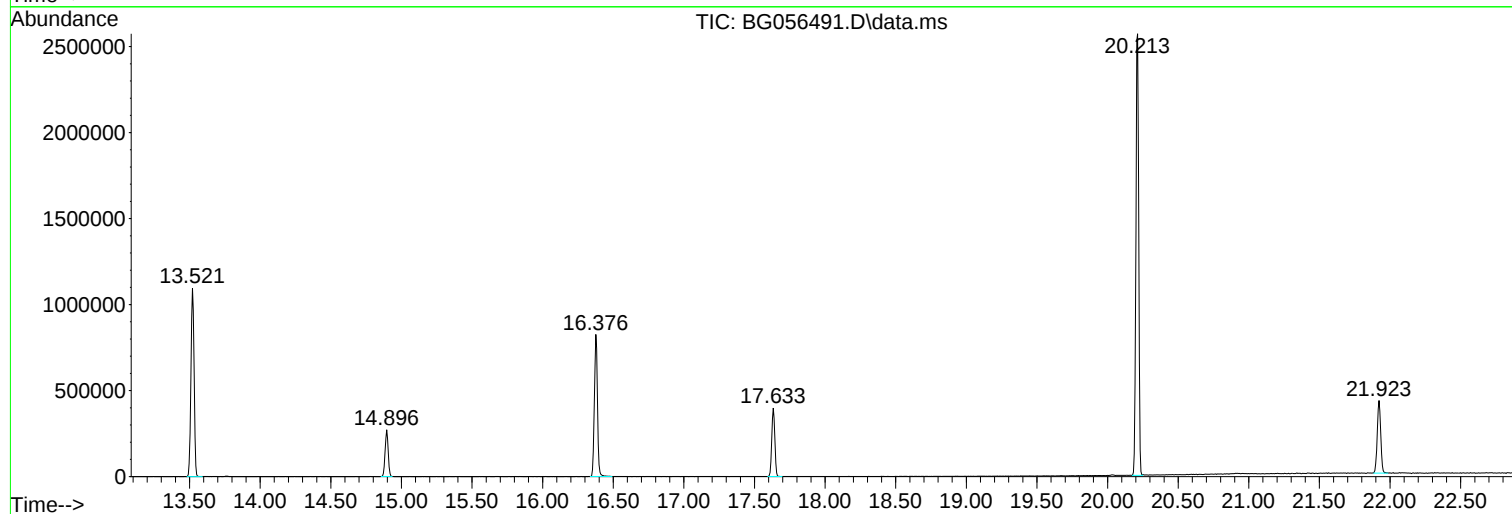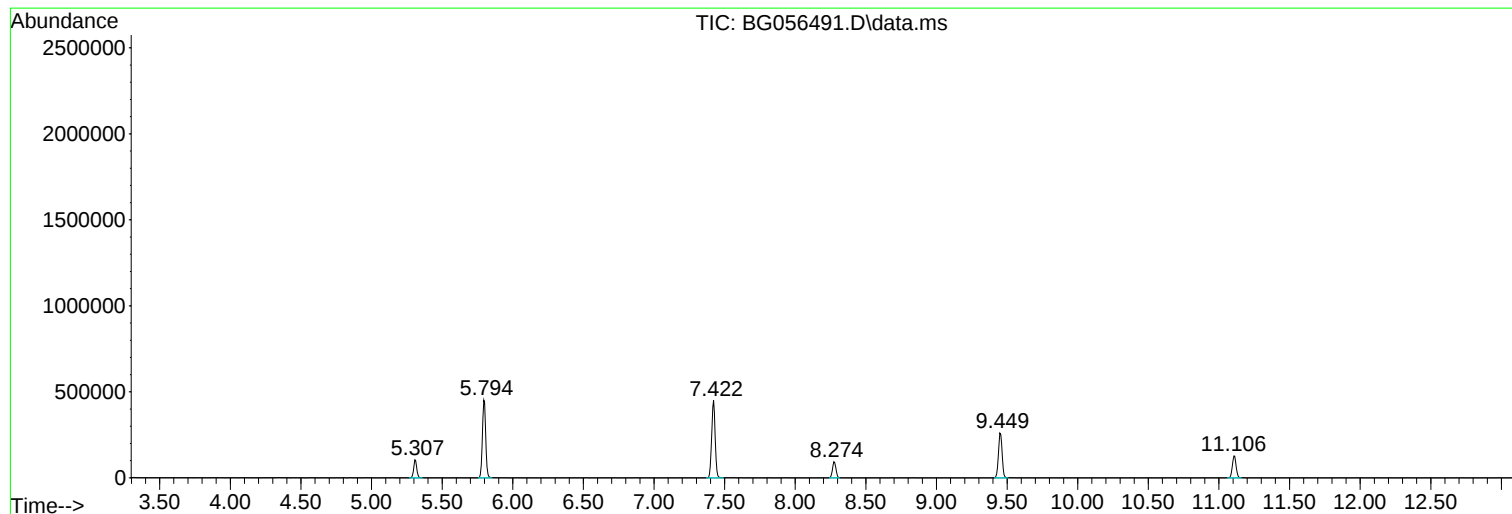

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013123\
Data File : BG056491.D
Acq On : 31 Jan 2023 18:56
Operator : CG/JU
Sample : PB150200BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150200BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.307 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.307	20.57 ng	158896	1,4-Dichlorobenzene-d4	8.274

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 1-ethoxy-2-methyl-	102	C6H14O	000627-02-1	35
2			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	33
3			3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	25
4			2,3-Dihydrooxazole, 2-t-butyl-4-...	98	C6H10O	036808-01-2	9
5			Methyl 1-methylcyclopropyl ketone	98	C6H10O	001567-75-5	9

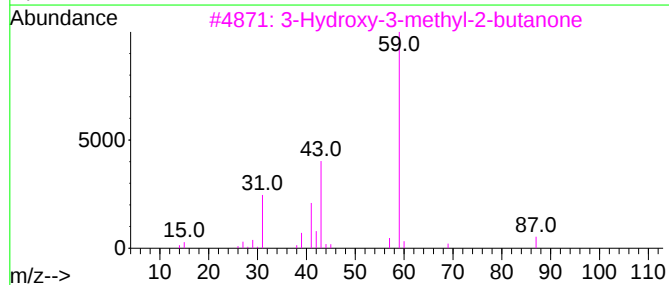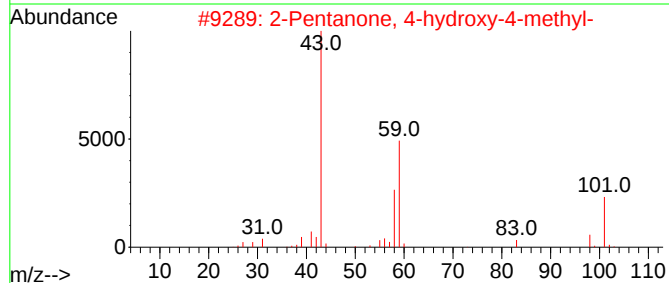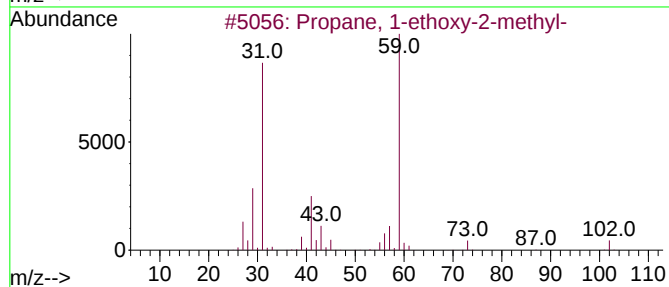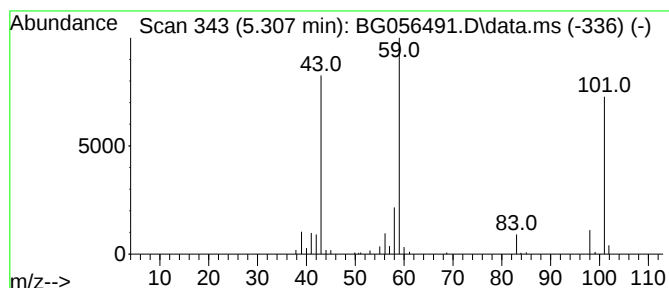

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013123\
Data File : BG056491.D
Acq On : 31 Jan 2023 18:56
Operator : CG/JU
Sample : PB150200BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150200BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.307	5.307	20.6	ng	158896	1	8.274	154516	20.0