


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013123\
 Data File : BG056478.D
 Acq On : 31 Jan 2023 9:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 01 01:15:52 2023

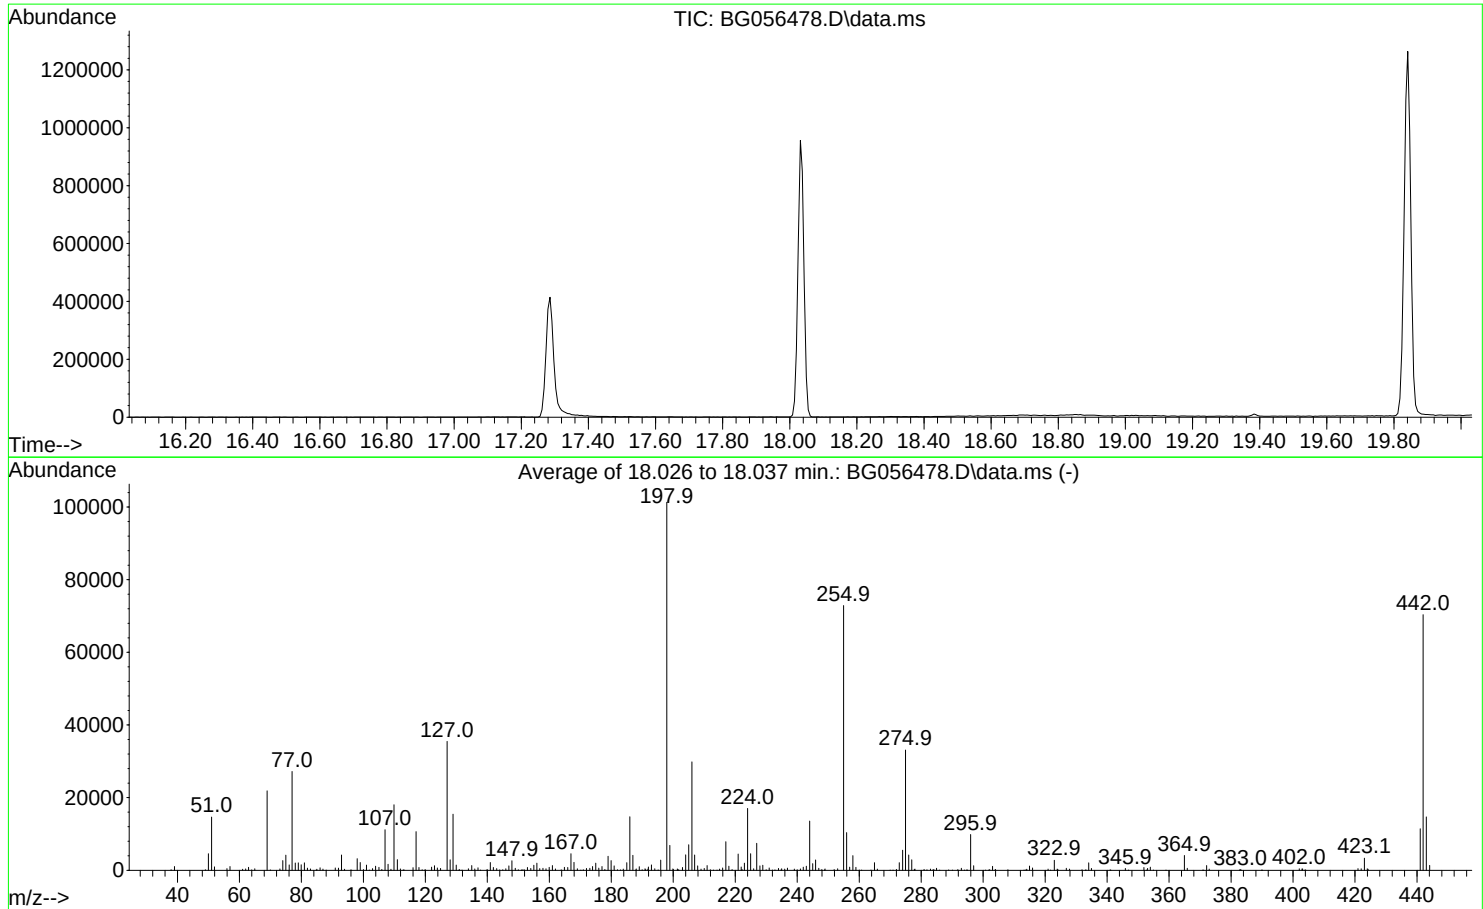




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	14.5	14648	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	21.6	21891	PASS
70	69	0.00	2	0.6	122	PASS
127	198	10	80	35.1	35504	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101272	PASS
199	198	5	9	6.8	6868	PASS
275	198	10	60	32.7	33099	PASS
365	198	1	100	4.0	4076	PASS
441	198	0.01	100	11.3	11430	PASS
442	442	50	100	100.0	70363	PASS
443	442	15	24	20.9	14686	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013123\
Data File : BG056478.D
Acq On : 31 Jan 2023 9:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 01 03:21:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:15:52 2023
Response via : Initial Calibration

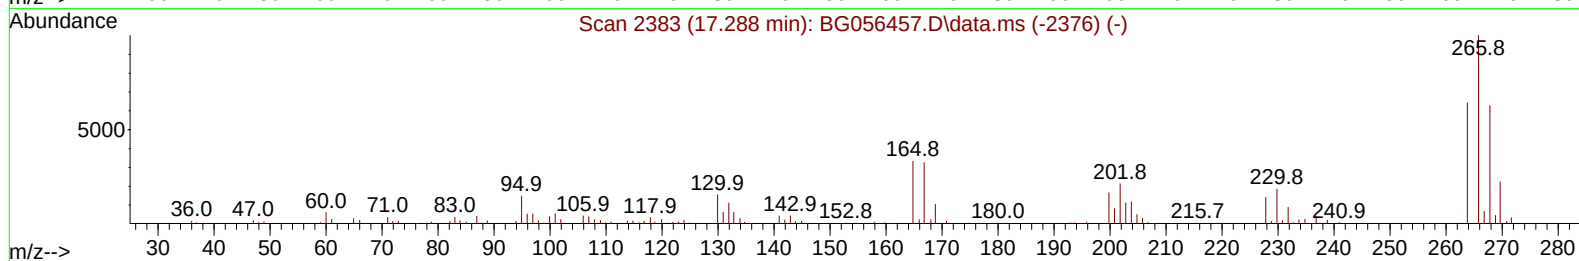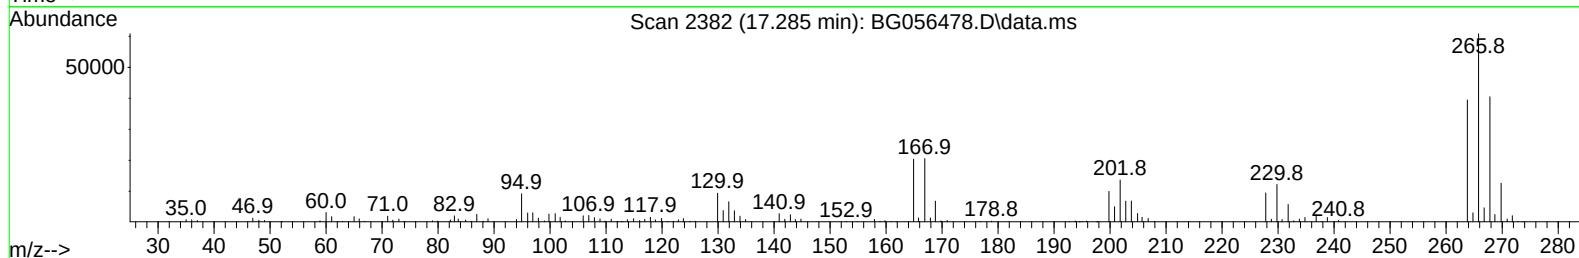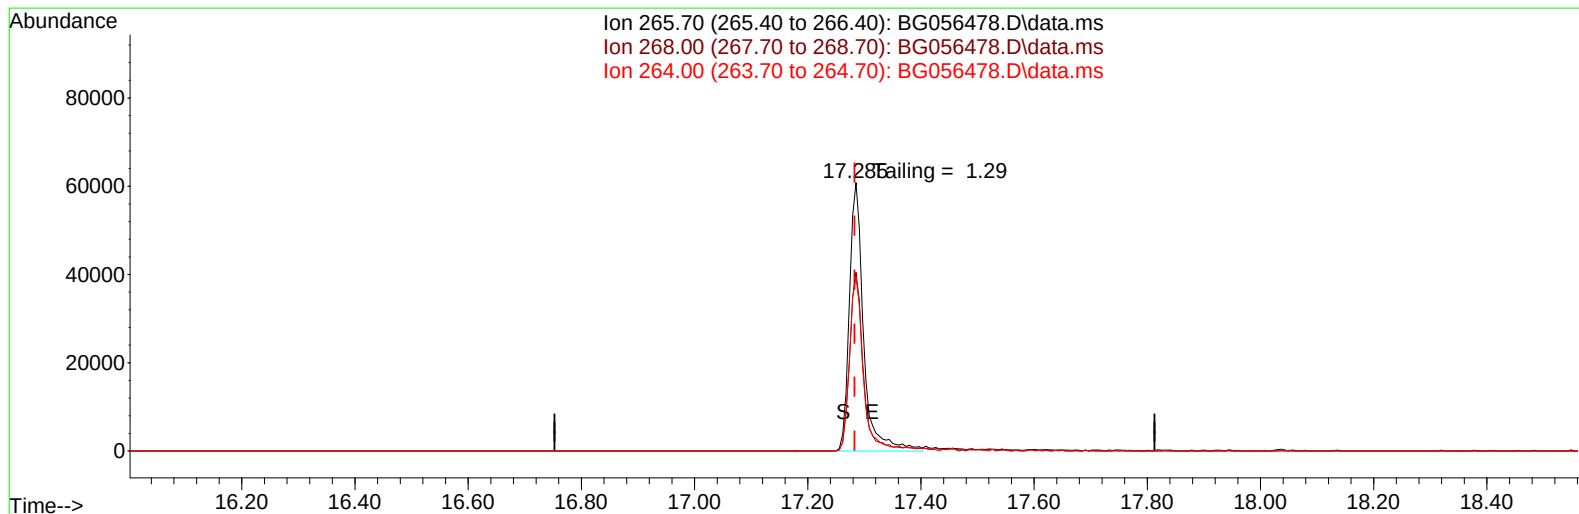

TIC: BG056478.D\data.ms

(70) Pentachlorophenol (C)

17.285min (+ 0.003) 22471.26 ng




response 106723

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	70.60
264.00	64.20	64.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013123\
Data File : BG056478.D
Acq On : 31 Jan 2023 9:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 01 03:21:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:15:52 2023
Response via : Initial Calibration

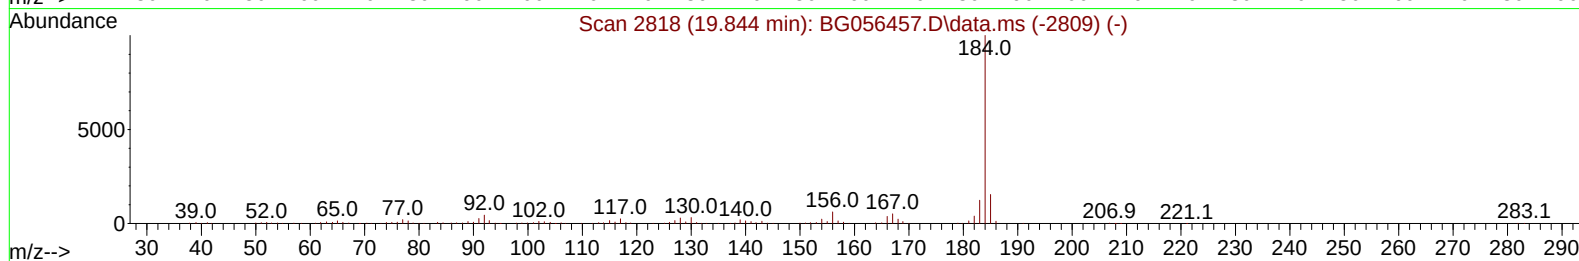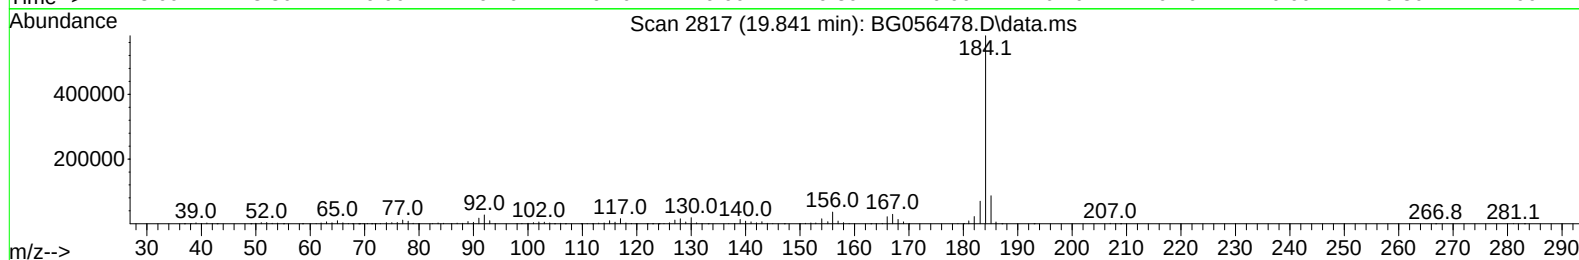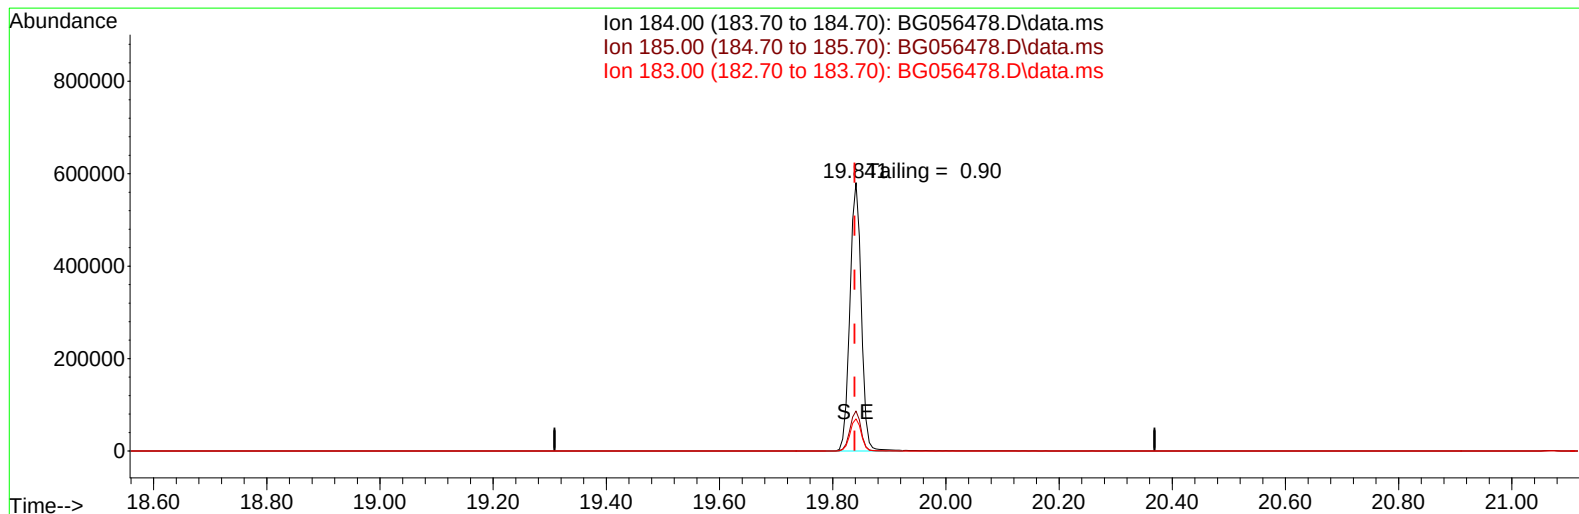

TIC: BG056478.D\data.ms

(77) Benzidine

19.841min (+ 0.003) 142958.10 ng

response 812410

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.90
183.00	12.30	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/31/2023	BNA_G	<u>BG056478.D</u>
Compound Name	Response	Retention Time
DDT	396763	21.069
DDD	9699	20.623
DDE	509	20.117
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10208	406971	2.51

Instrument :
BNA_G
ClientSampleId :
DFTPP