


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013124\
Data File : BG060504.D
Acq On : 31 Jan 2024 11:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

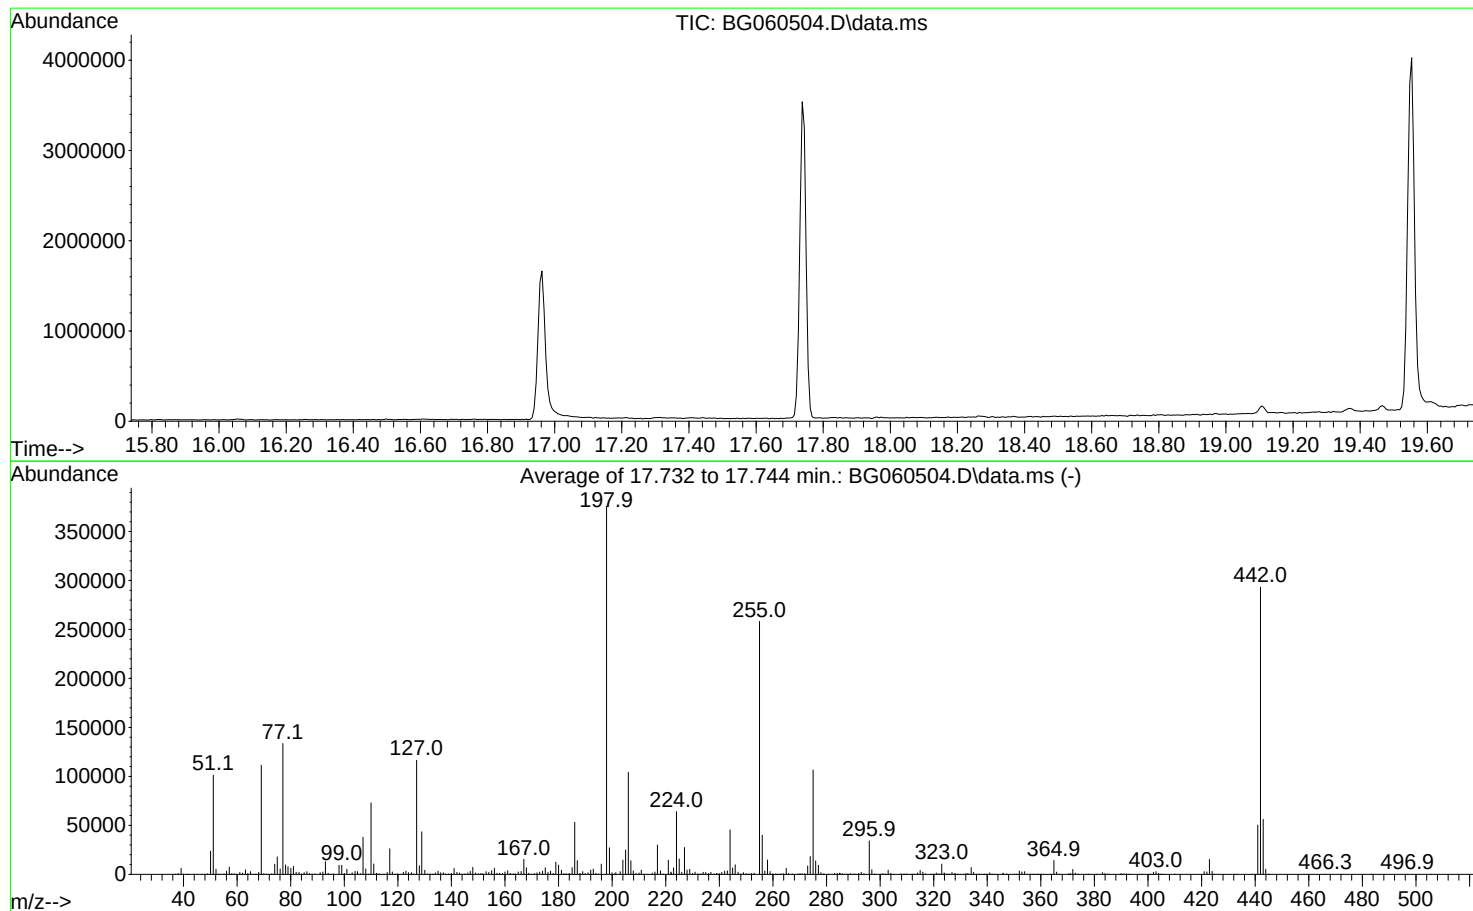




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	101229	PASS
68	69	0.00	2	1.9	2065	PASS
69	198	0.00	100	29.7	111436	PASS
70	69	0.00	2	0.6	693	PASS
127	198	10	80	31.0	116488	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	375659	PASS
199	198	5	9	7.2	27075	PASS
275	198	10	60	28.3	106384	PASS
365	198	1	100	3.8	14223	PASS
441	198	0.01	100	13.4	50181	PASS
442	442	50	100	100.0	293184	PASS
443	442	15	24	19.2	56179	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013124\
Data File : BG060504.D
Acq On : 31 Jan 2024 11:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 01 00:41:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

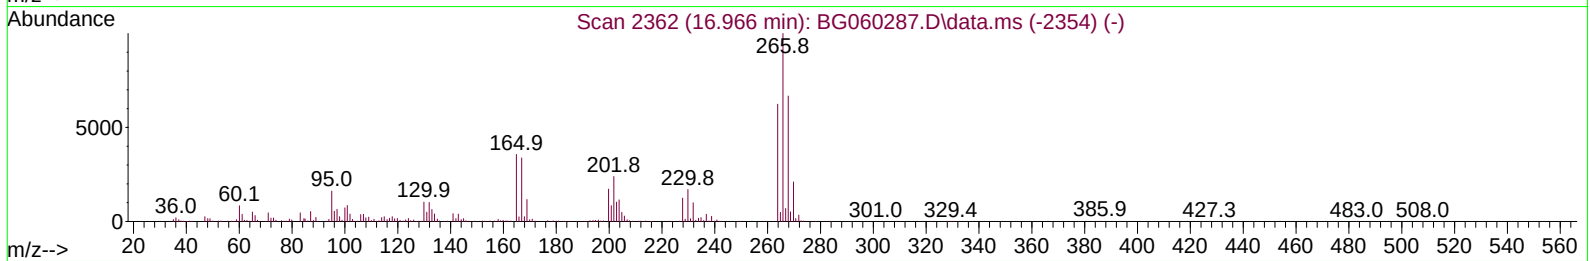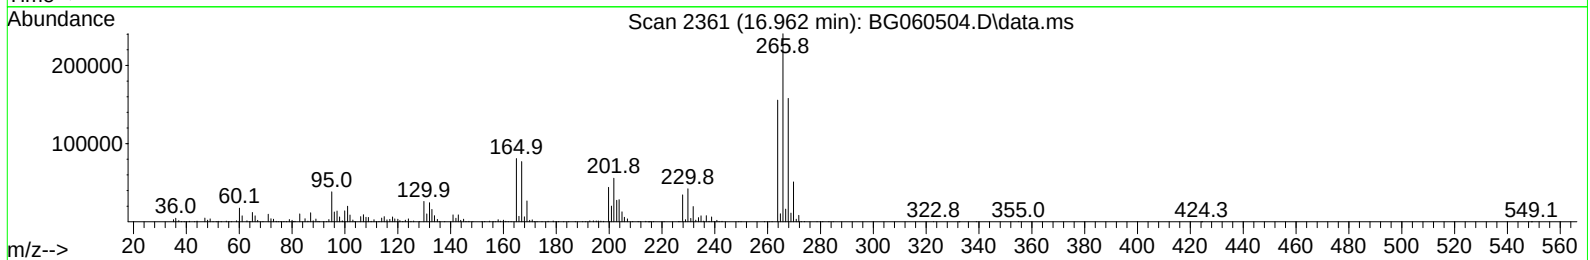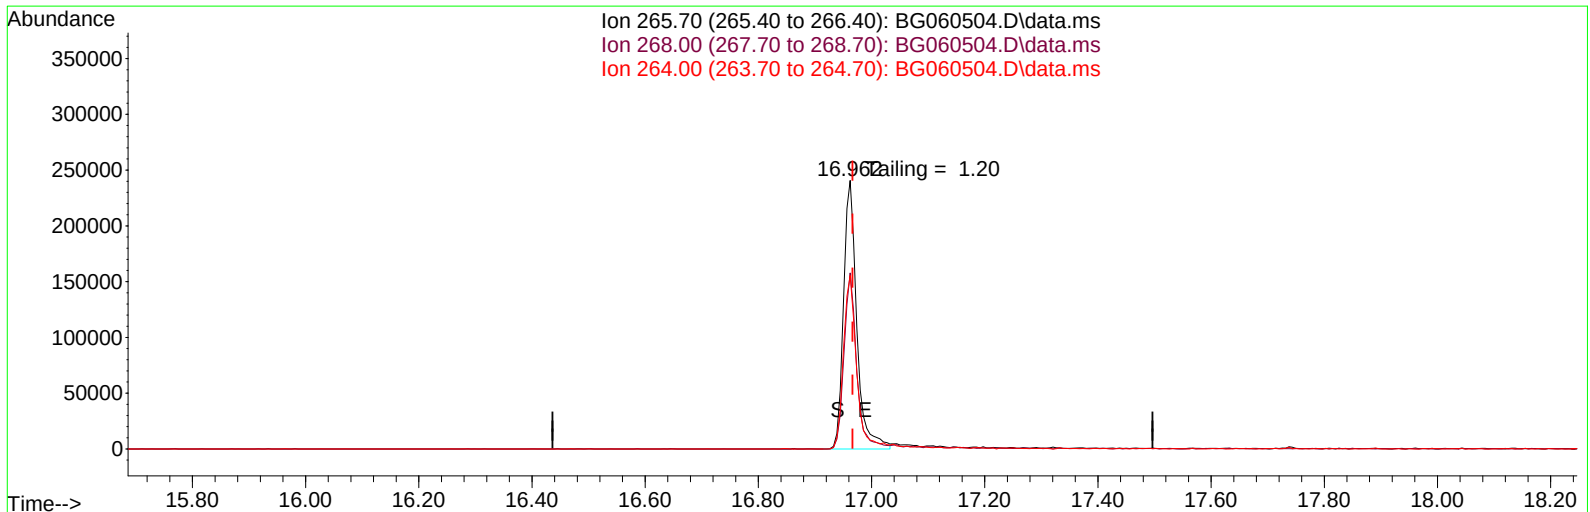

TIC: BG060504.D\data.ms

(70) Pentachlorophenol (C)

16.962min (-0.004) 108145.45 ng




response 403357

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	65.56
264.00	62.30	64.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG013124\
Data File : BG060504.D
Acq On : 31 Jan 2024 11:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 01 00:41:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

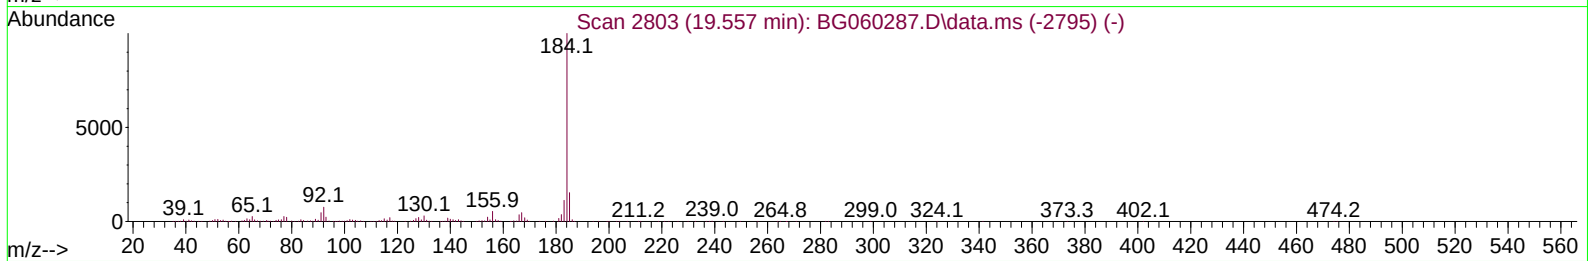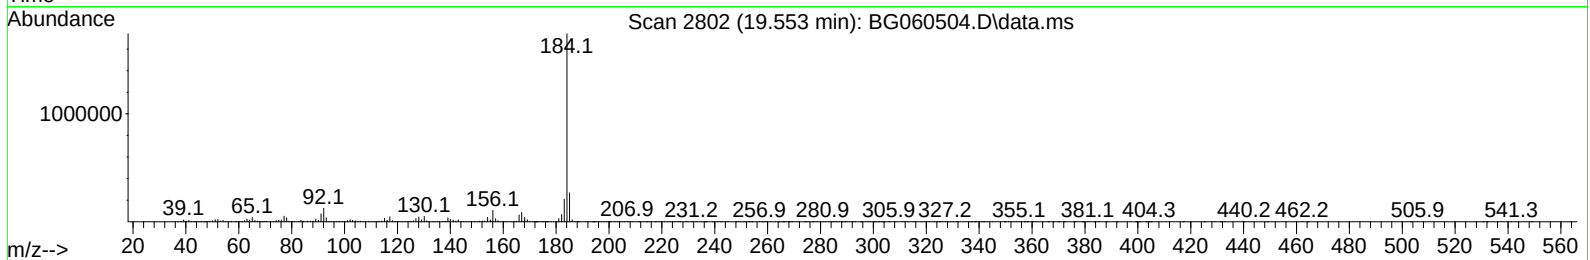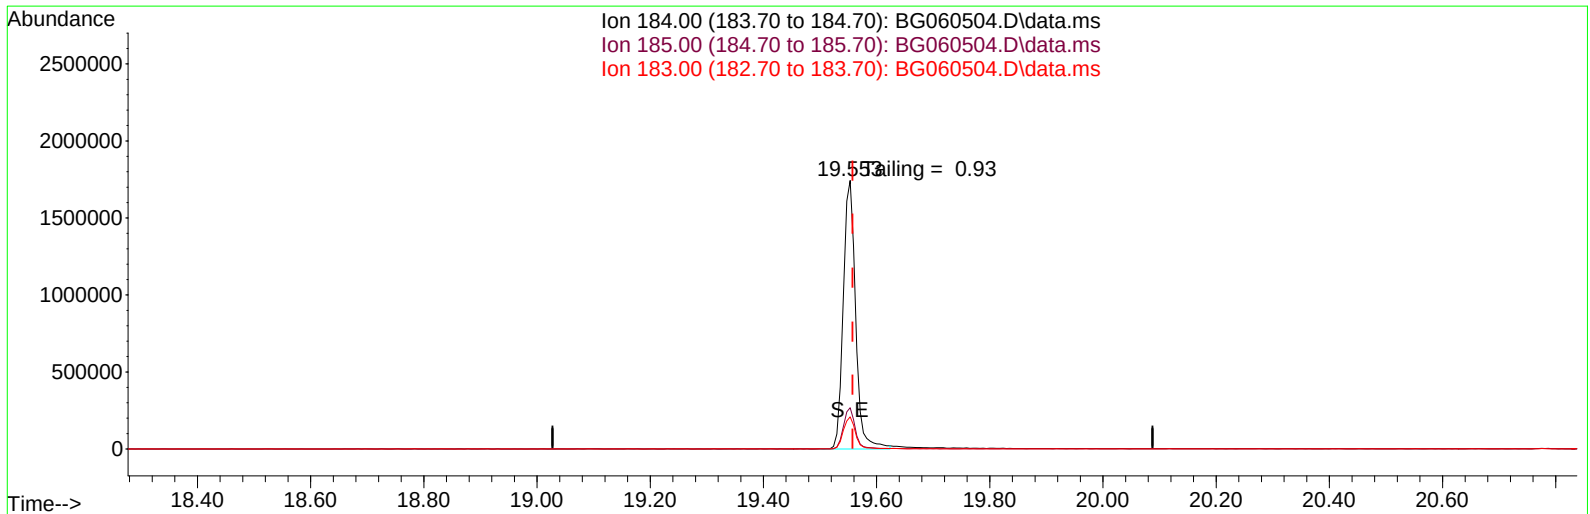

TIC: BG060504.D\data.ms

(77) Benzidine

19.553min (-0.004) 284106.29 ng

response 2678764

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	15.38
183.00	11.20	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/31/2024	BNA_G	<u>BG060504.D</u>
Compound Name	Response	Retention Time
DDT	1129201	20.781
DDD	146769	20.341
DDE	1903	19.829
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
148672	1277873	11.63

Instrument :
BNA_G
ClientSampleId :
DFTPP