

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020116\
 Data File : BG020773.D
 Acq On : 1 Feb 2016 14:51
 Operator : SJ/IZ
 Sample : PB88049BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK49

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG012716.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	67	72	82	rVB	16771	29877	6.16%	0.619%
2	3.339	82	85	92	rVB4	2187	3547	0.73%	0.074%
3	3.392	92	94	96	rBV3	608	589	0.12%	0.012%
4	3.427	98	100	103	rBV4	441	576	0.12%	0.012%
5	3.615	127	132	138	rVB3	3482	4860	1.00%	0.101%
6	3.756	153	156	161	rVB3	492	880	0.18%	0.018%
7	3.797	161	163	165	rBV2	527	676	0.14%	0.014%
8	3.868	173	175	178	rVB3	572	556	0.11%	0.012%
9	4.291	245	247	252	rVB2	452	579	0.12%	0.012%
10	5.460	444	446	449	rBV2	485	694	0.14%	0.014%
11	5.589	465	468	471	rVV2	443	676	0.14%	0.014%
12	6.323	588	593	594	rVV2	454	654	0.13%	0.014%
13	6.347	594	597	600	rVB3	505	617	0.13%	0.013%
14	7.122	725	729	731	rBV2	597	715	0.15%	0.015%
15	7.410	771	778	787	rBV	56681	92220	19.00%	1.912%
16	7.592	802	809	817	rBV	58342	96118	19.80%	1.992%
17	7.692	824	826	830	rBV2	407	714	0.15%	0.015%
18	7.804	837	845	852	rBV	57060	96320	19.85%	1.997%
19	8.279	919	926	932	rVB	53319	86427	17.81%	1.792%
20	8.479	956	960	963	rVB2	569	789	0.16%	0.016%
21	8.720	999	1001	1003	rBV2	742	739	0.15%	0.015%
22	8.849	1019	1023	1027	rVB	441	816	0.17%	0.017%
23	8.967	1037	1043	1051	rVV	79783	131872	27.17%	2.734%
24	9.448	1115	1125	1133	rBV	52047	92357	19.03%	1.915%
25	9.589	1146	1149	1152	rBV2	500	643	0.13%	0.013%
26	9.648	1156	1159	1162	rVB	721	927	0.19%	0.019%
27	9.695	1162	1167	1170	rBB2	543	1070	0.22%	0.022%
28	9.730	1170	1173	1176	rBV2	684	1009	0.21%	0.021%
29	10.171	1239	1248	1256	rBV	28046	49211	10.14%	1.020%
30	10.412	1288	1289	1294	rBV2	416	616	0.13%	0.013%
31	10.711	1333	1340	1348	rVB	67759	117108	24.13%	2.428%
32	11.105	1399	1407	1414	rBV	83998	152155	31.35%	3.154%
33	11.228	1421	1428	1437	rVB	90471	156860	32.32%	3.252%
34	11.598	1488	1491	1494	rBV	573	797	0.16%	0.017%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020116\
 Data File : BG020773.D
 Acq On : 1 Feb 2016 14:51
 Operator : SJ/IZ
 Sample : PB88049BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK49

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG012716.M
 Title : SVOA CALIBRATION

35	11.963	1549	1553	1556	rVV2	495	812	0.17%	0.017%
36	12.145	1581	1584	1588	rVB	559	857	0.18%	0.018%
37	12.286	1604	1608	1611	rBV2	616	874	0.18%	0.018%
38	12.403	1627	1628	1631	rBB	586	572	0.12%	0.012%
39	12.662	1669	1672	1676	rVB	1166	1479	0.30%	0.031%
40	13.443	1801	1805	1807	rVB	414	681	0.14%	0.014%
41	13.837	1870	1872	1876	rBV	688	765	0.16%	0.016%
42	13.884	1876	1880	1885	rVV	277	562	0.12%	0.012%
43	14.283	1942	1948	1956	rVB	182546	257969	53.15%	5.348%
44	14.447	1974	1976	1980	rBV	357	667	0.14%	0.014%
45	14.583	1992	1999	2006	rVV	196301	315367	64.98%	6.537%
46	14.888	2044	2051	2058	rVB2	148260	231739	47.75%	4.804%
47	15.047	2072	2078	2088	rBV	68453	103835	21.39%	2.152%
48	15.158	2094	2097	2100	rVB	417	650	0.13%	0.013%
49	15.810	2203	2208	2211	rVB	476	912	0.19%	0.019%
50	15.875	2211	2219	2227	rBV	272564	411083	84.70%	8.522%
51	15.969	2231	2235	2241	rVV	28491	39185	8.07%	0.812%
52	16.116	2256	2260	2263	rBV3	1951	2255	0.46%	0.047%
53	17.402	2475	2479	2481	rBV2	601	802	0.17%	0.017%
54	17.490	2489	2494	2496	rVB	481	660	0.14%	0.014%
55	17.620	2510	2516	2526	rVB2	190647	287687	59.27%	5.964%
56	17.720	2526	2533	2540	rBV2	305023	445353	91.76%	9.232%
57	17.984	2575	2578	2583	rVB2	598	748	0.15%	0.016%
58	18.066	2587	2592	2595	rBV3	357	746	0.15%	0.015%
59	18.342	2638	2639	2644	rVB3	416	655	0.13%	0.014%
60	18.554	2672	2675	2680	rBV2	605	978	0.20%	0.020%
61	18.930	2733	2739	2740	rBV2	469	821	0.17%	0.017%
62	19.623	2853	2857	2861	rBV	2813	3858	0.79%	0.080%
63	19.828	2889	2892	2893	rBV	562	576	0.12%	0.012%
64	19.870	2897	2899	2905	rVB2	1748	2313	0.48%	0.048%
65	19.917	2905	2907	2910	rVB2	623	609	0.13%	0.013%
66	19.987	2912	2919	2925	rVV2	331365	485352	100.00%	10.061%
67	20.181	2948	2952	2953	rBV2	554	571	0.12%	0.012%
68	20.269	2964	2967	2968	rBV	769	880	0.18%	0.018%
69	20.351	2978	2981	2983	rBV3	662	845	0.17%	0.018%
70	20.392	2987	2988	2991	rBV2	679	613	0.13%	0.013%
71	20.486	3002	3004	3005	rBV	812	705	0.15%	0.015%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020116\
 Data File : BG020773.D
 Acq On : 1 Feb 2016 14:51
 Operator : SJ/IZ
 Sample : PB88049BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK49

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG012716.M
 Title : SVOA CALIBRATION

72	20.516	3007	3009	3011	rBV2	972	708	0.15%	0.015%
73	20.809	3057	3059	3061	rBV3	783	679	0.14%	0.014%
74	21.021	3094	3095	3098	rBV2	614	657	0.14%	0.014%
75	21.456	3167	3169	3170	rBV	854	602	0.12%	0.012%
76	21.526	3178	3181	3182	rBV3	1664	1153	0.24%	0.024%
77	21.902	3238	3245	3252	rVB	190483	298773	61.56%	6.193%
78	22.102	3275	3279	3281	rBV3	1697	1617	0.33%	0.034%
79	22.595	3361	3363	3364	rBV2	811	618	0.13%	0.013%
80	23.382	3495	3497	3498	rBV	910	689	0.14%	0.014%
81	23.471	3509	3512	3516	rBV6	1574	2846	0.59%	0.059%
82	23.670	3544	3546	3548	rBV3	708	699	0.14%	0.014%
83	23.888	3581	3583	3587	rBV3	952	1155	0.24%	0.024%
84	24.105	3616	3620	3624	rVB6	1472	2880	0.59%	0.060%
85	24.334	3654	3659	3666	rVB5	3997	8136	1.68%	0.169%
86	24.405	3669	3671	3675	rBV3	806	981	0.20%	0.020%
87	25.051	3770	3781	3793	rVB	167858	458154	94.40%	9.497%
88	25.180	3802	3803	3808	rBV5	836	1136	0.23%	0.024%
89	25.215	3808	3809	3810	rVV	1574	812	0.17%	0.017%
90	25.286	3810	3821	3839	rVB2	97449	291950	60.15%	6.052%
91	26.138	3964	3966	3971	rBV4	935	1595	0.33%	0.033%
92	26.302	3992	3994	3997	rBV4	952	692	0.14%	0.014%
93	26.555	4030	4037	4044	rVB7	4711	12674	2.61%	0.263%
94	27.612	4215	4217	4220	rVB3	1130	1116	0.23%	0.023%
95	28.188	4313	4315	4317	rBV3	786	719	0.15%	0.015%
96	30.103	4639	4641	4642	rBV2	988	608	0.13%	0.013%
97	31.031	4797	4799	4800	rBV2	991	726	0.15%	0.015%
98	31.143	4816	4818	4819	rBV2	872	667	0.14%	0.014%
99	31.489	4875	4877	4879	rBV2	900	869	0.18%	0.018%
100	31.648	4902	4904	4907	rBV4	914	795	0.16%	0.016%


Sum of corrected areas: 4824006

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020116\
Data File : BG020773.D
Acq On : 1 Feb 2016 14:51
Operator : SJ/IZ
Sample : PB88049BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK49

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG012716.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

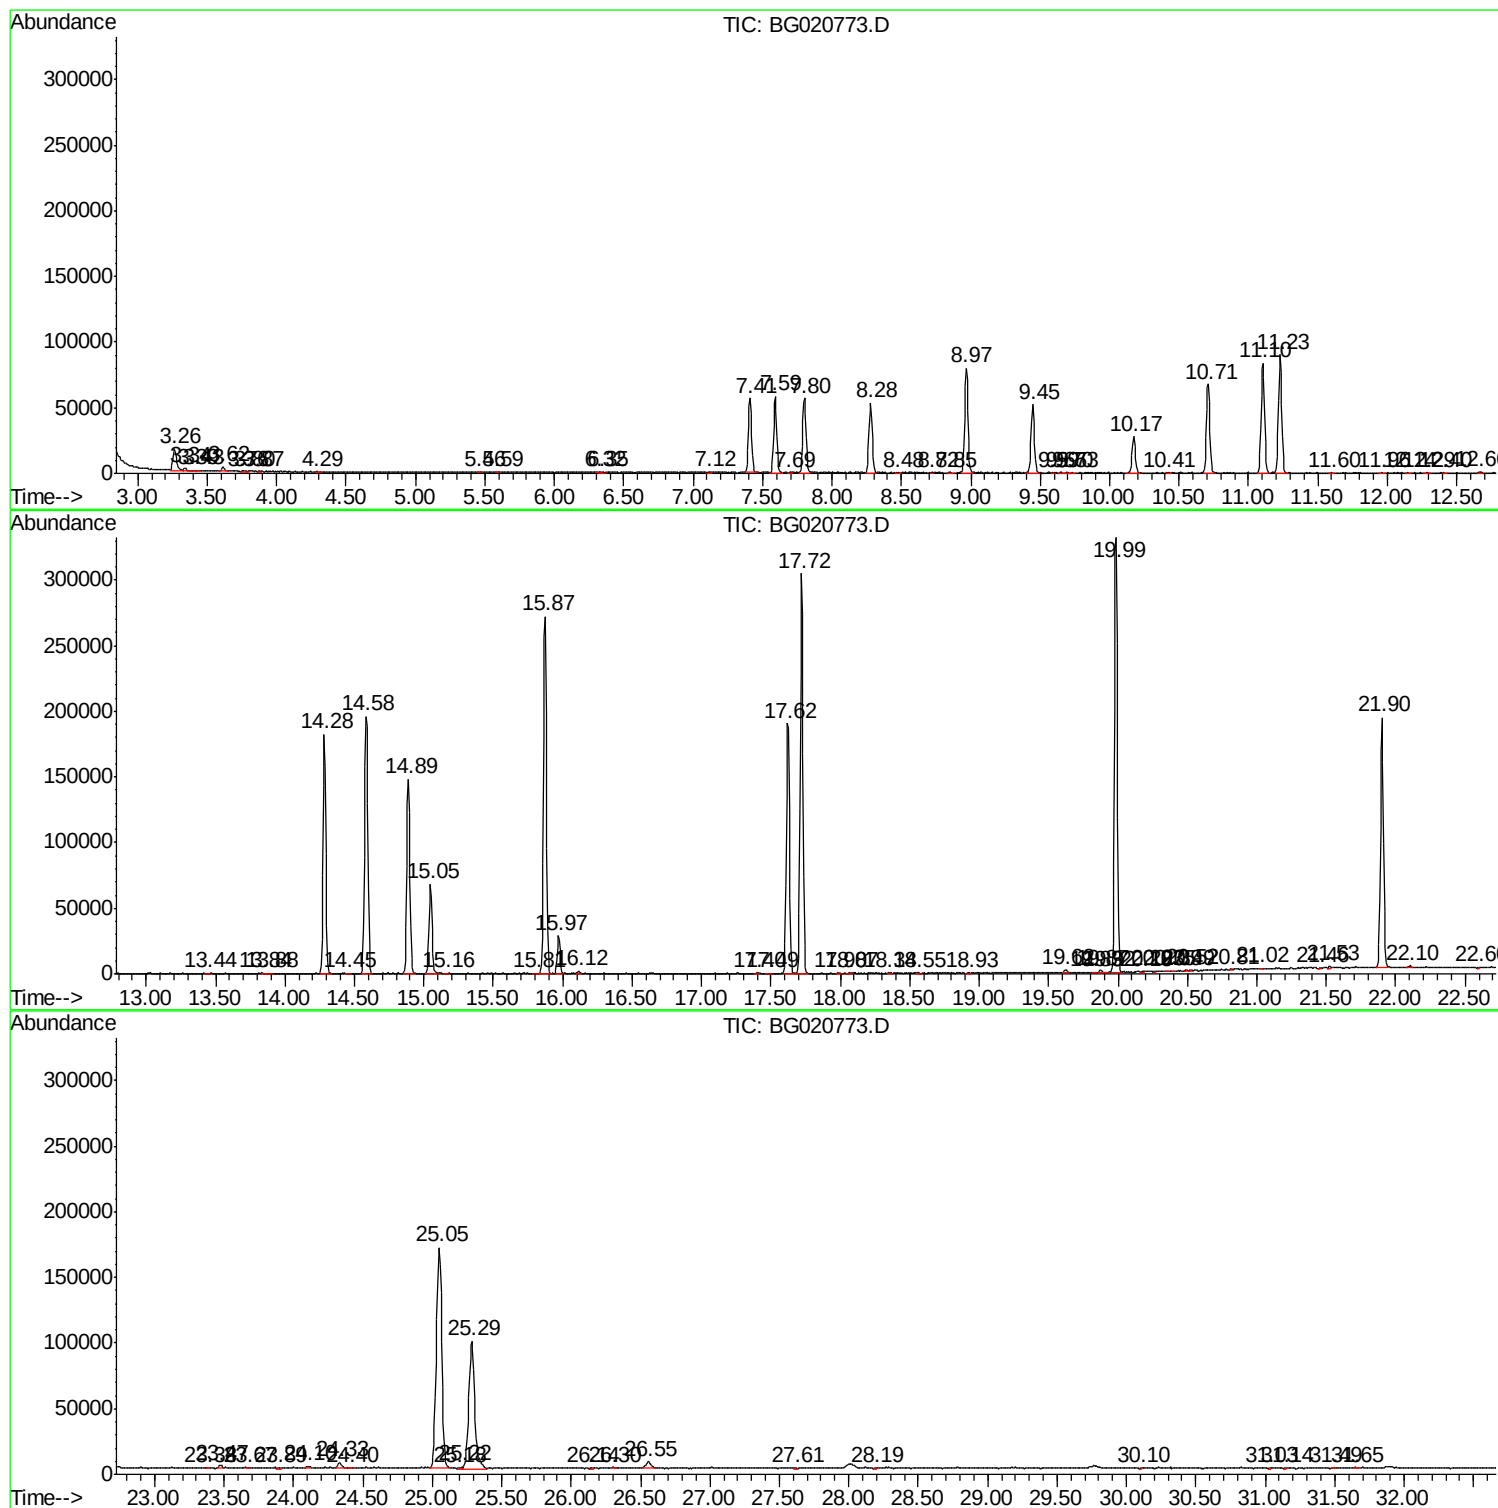

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020116\
Data File : BG020773.D
Acq On : 1 Feb 2016 14:51
Operator : SJ/IZ
Sample : PB88049BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK49

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG012716.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020116\
Data File : BG020773.D
Acq On : 1 Feb 2016 14:51
Operator : SJ/IZ
Sample : PB88049BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK49

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG012716.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc