


Data Path : Z:\HPCHEM1\BNA G\Data\BG020118\
 Data File : BG032487.D
 Acq On : 1 Feb 2018 13:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 29 15:32:55 2018

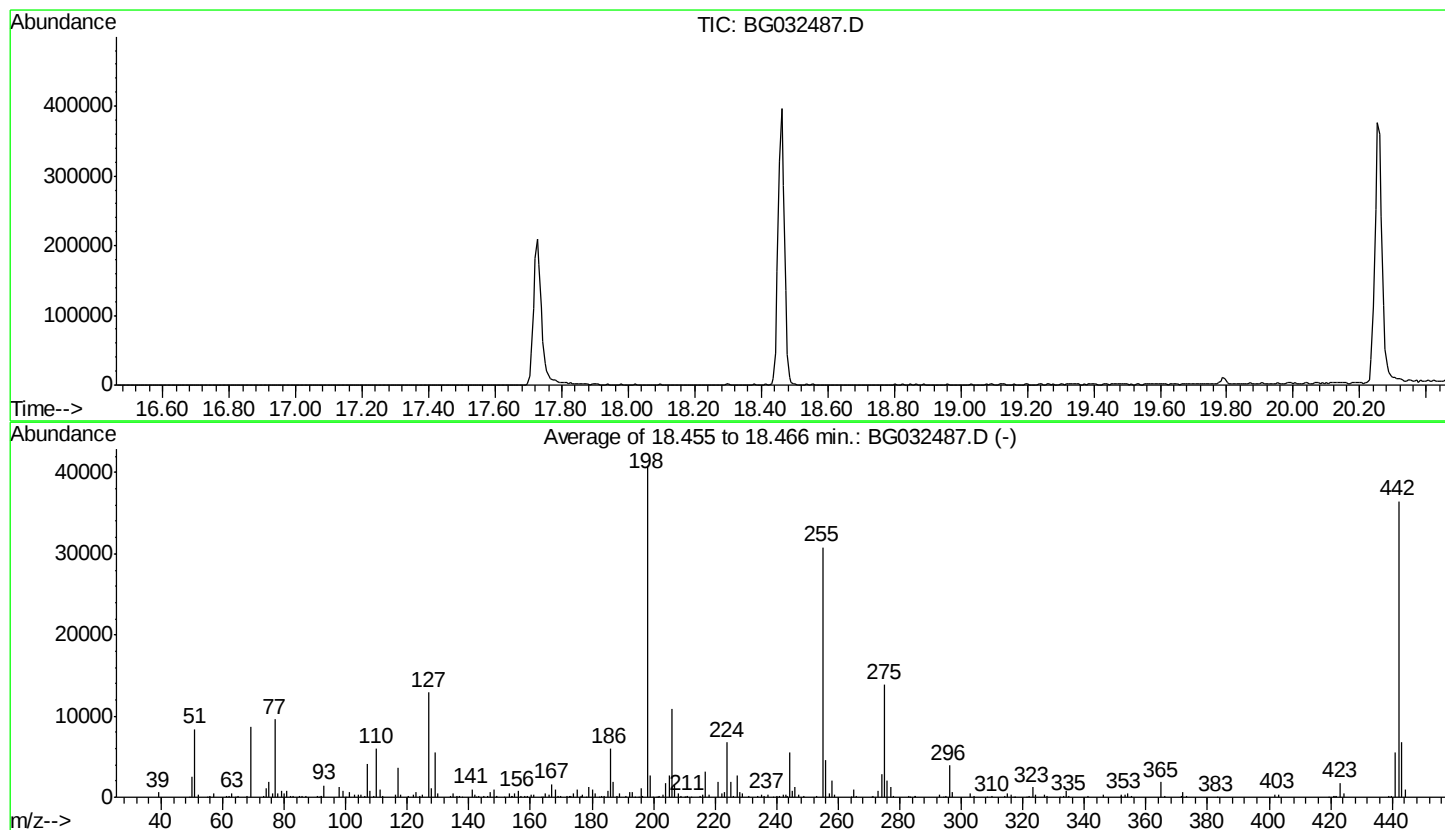

AutoFind: Scans 2581, 2582, 2583; Background Corrected with Scan 2574

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.6	8413	PASS
68	69	0.00	2	1.4	123	PASS
69	198	0.00	100	21.2	8652	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.6	12920	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40861	PASS
199	198	5	9	6.8	2763	PASS
275	198	10	60	33.9	13843	PASS
365	198	1	100	4.5	1843	PASS
441	442	0.01	24	15.1	5506	PASS
442	198	50	100	89.3	36485	PASS
443	442	15	24	18.8	6844	PASS