




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
 Data File : BG060526.D
 Acq On : 1 Feb 2024 3:19
 Operator : MA/JU
 Sample : PB158739BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK739

Manual IntegrationsAPPROVED

Quant Time: Feb 01 03:55:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 31 22:04:13 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/01/2024
 Supervised By :Sohil Jodhani 02/02/2024

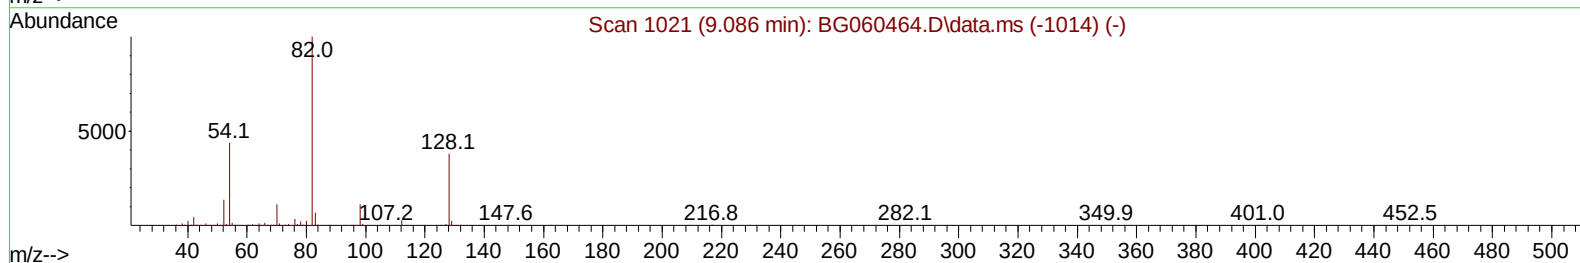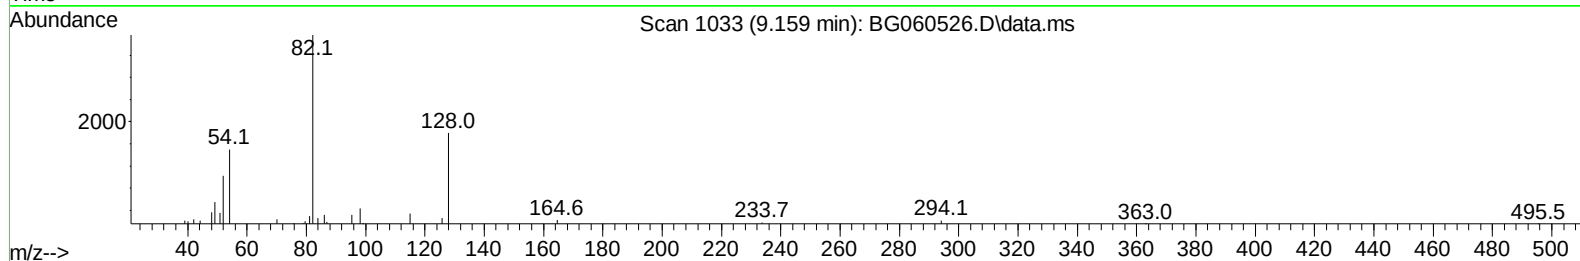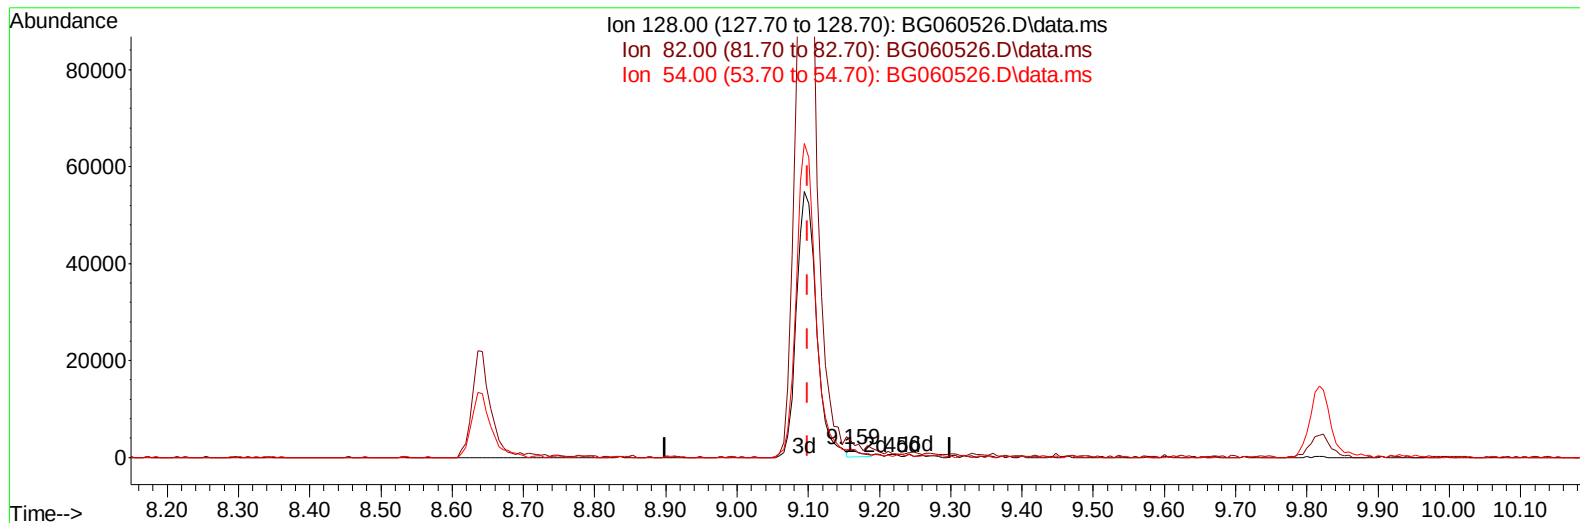

TIC: BG060526.D\data.ms

(21) Nitrobenzene-d5 (S)

9.159min (+ 0.060) 0.56 ng/u1

response 1821

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	238.70	198.22
54.00	95.30	83.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
 Data File : BG060526.D
 Acq On : 1 Feb 2024 3:19
 Operator : MA/JU
 Sample : PB158739BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK739

Manual IntegrationsAPPROVED

Quant Time: Feb 01 03:55:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 31 22:04:13 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/01/2024
 Supervised By :Sohil Jodhani 02/02/2024

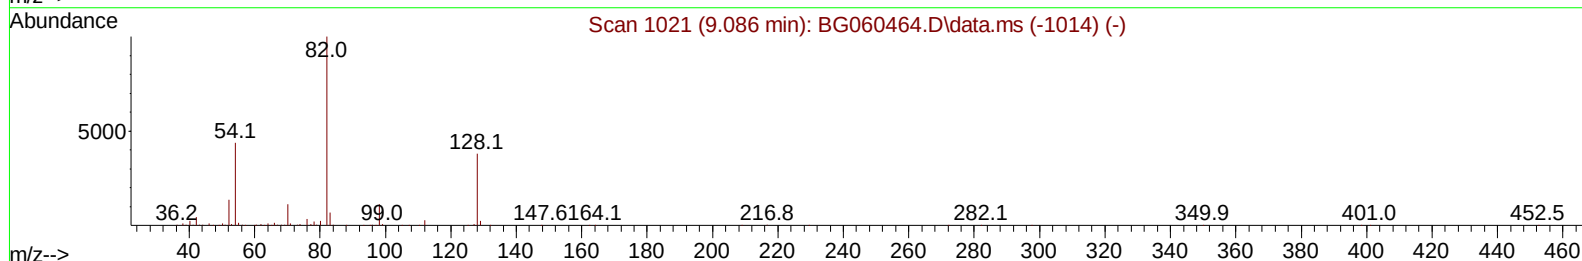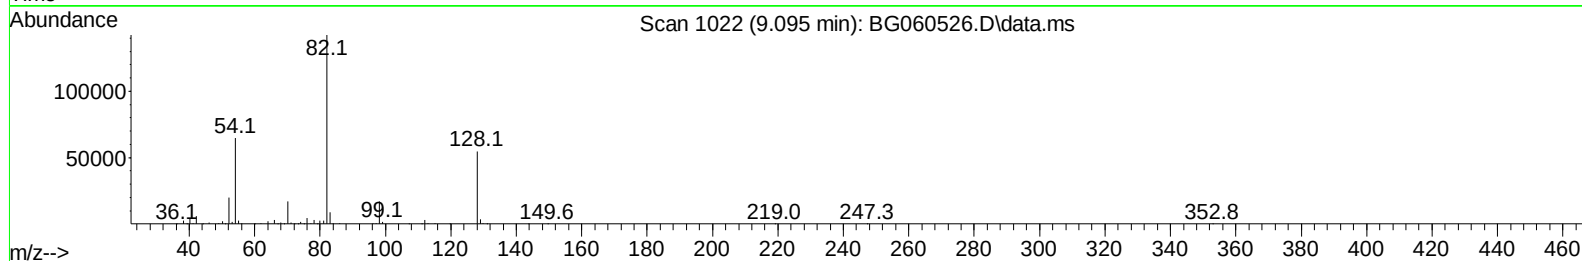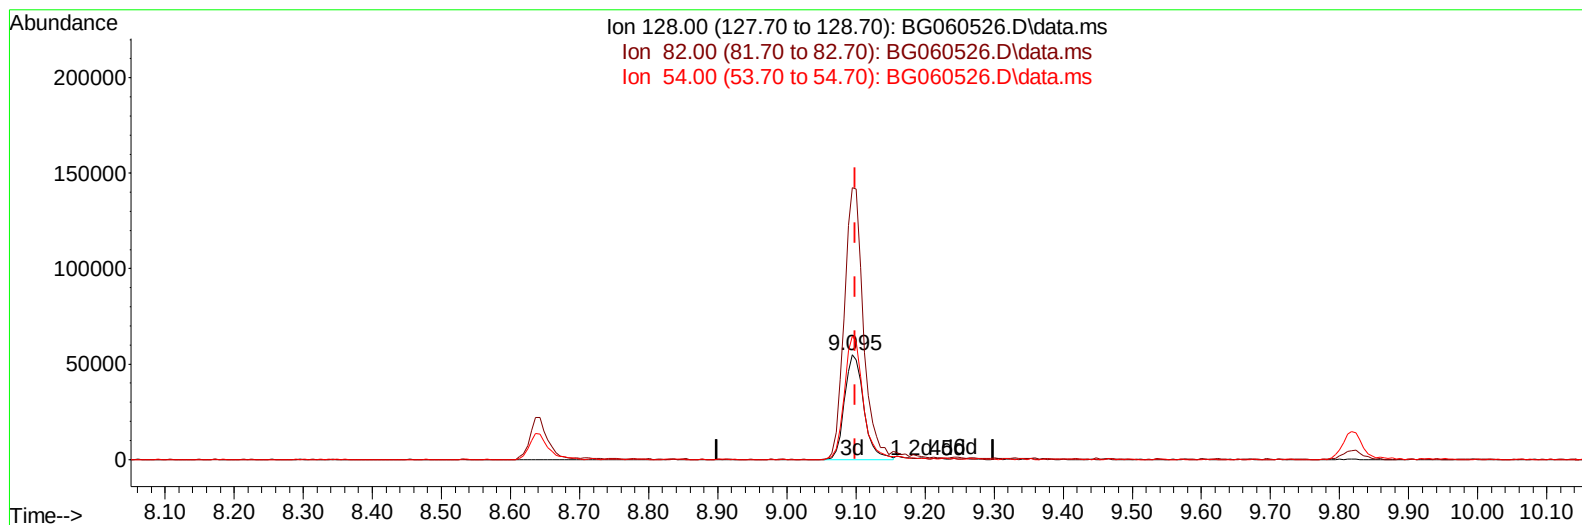

TIC: BG060526.D\data.ms

(21) Nitrobenzene-d5 (S)

9.095min (-0.004) 32.36 ng/ul m

response 105854

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	238.70	259.43
54.00	95.30	118.03#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
 Data File : BG060526.D
 Acq On : 1 Feb 2024 3:19
 Operator : MA/JU
 Sample : PB158739BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK739

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/01/2024
 Supervised By :Sohil Jodhani 02/02/2024

Quant Time: Feb 01 03:56:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 31 22:04:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.937	152	103442	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	443425	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.571	164	391750	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.320	188	1096238	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	1055673	20.000	ng/ul	0.00
88) Perylene-d12	24.747	264	1188761	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	16974	8.223	ng/uL	0.00
4) Pyridine-d5	3.783	84	195474	29.934	ng/ul	0.00
7) Phenol-d5	7.097	99	274083	27.899	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.256	67	168687	27.324	ng/ul	0.00
11) 2-Chlorophenol-d4	7.467	132	187310	28.551	ng/ul	0.00
15) 4-Methylphenol-d8	8.642	113	228376	28.221	ng/ul	0.00
21) Nitrobenzene-d5	9.095	128	105854m	32.361	ng/ul	0.00
24) 2-Nitrophenol-d4	9.823	143	132316	34.623	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.358	165	264752	33.311	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	326061	31.273	ng/ul	0.00
46) Dimethylphthalate-d6	13.971	166	1045306	32.609	ng/ul	0.00
49) Acenaphthylene-d8	14.265	160	1144269	31.823	ng/ul	0.00
54) 4-Nitrophenol-d4	14.770	143	130916	28.514	ng/ul	0.00
60) Fluorene-d10	15.564	176	953693	33.954	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	155101	22.849	ng/ul	0.00
73) Anthracene-d10	17.414	188	1714819	32.999	ng/ul	0.00
81) Pyrene-d10	19.706	212	2110880	33.362	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.535	264	2037715	32.677	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060526.D
Acq On : 1 Feb 2024 3:19
Operator : MA/JU
Sample : PB158739BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK739

Manual IntegrationsAPPROVED

Quant Time: Feb 01 03:56:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 31 22:04:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/01/2024
Supervised By :Sohil Jodhani 02/02/2024

