




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060527.D
Acq On : 1 Feb 2024 4:00
Operator : MA/JU
Sample : P1289-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 04:33:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 31 22:04:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/01/2024
Supervised By :Sohil Jodhani 02/02/2024

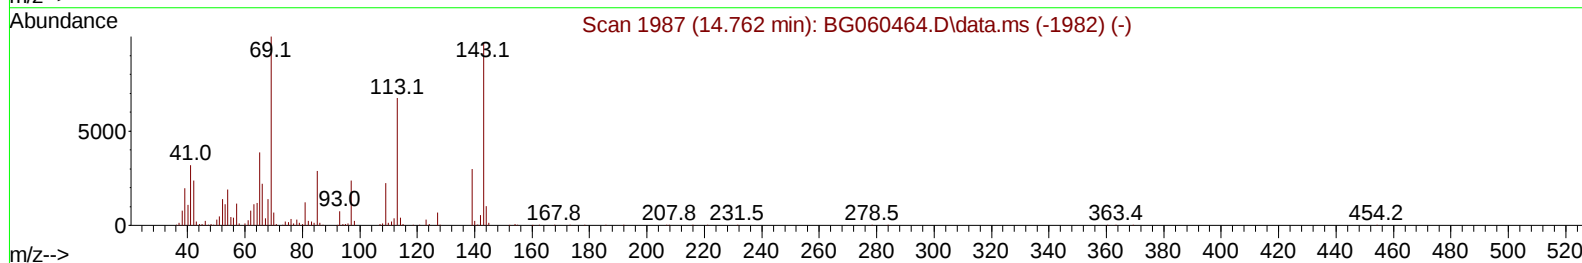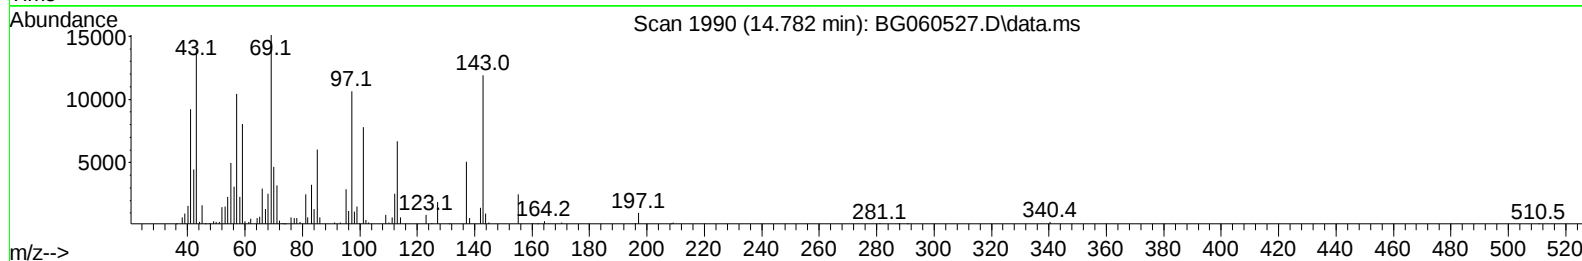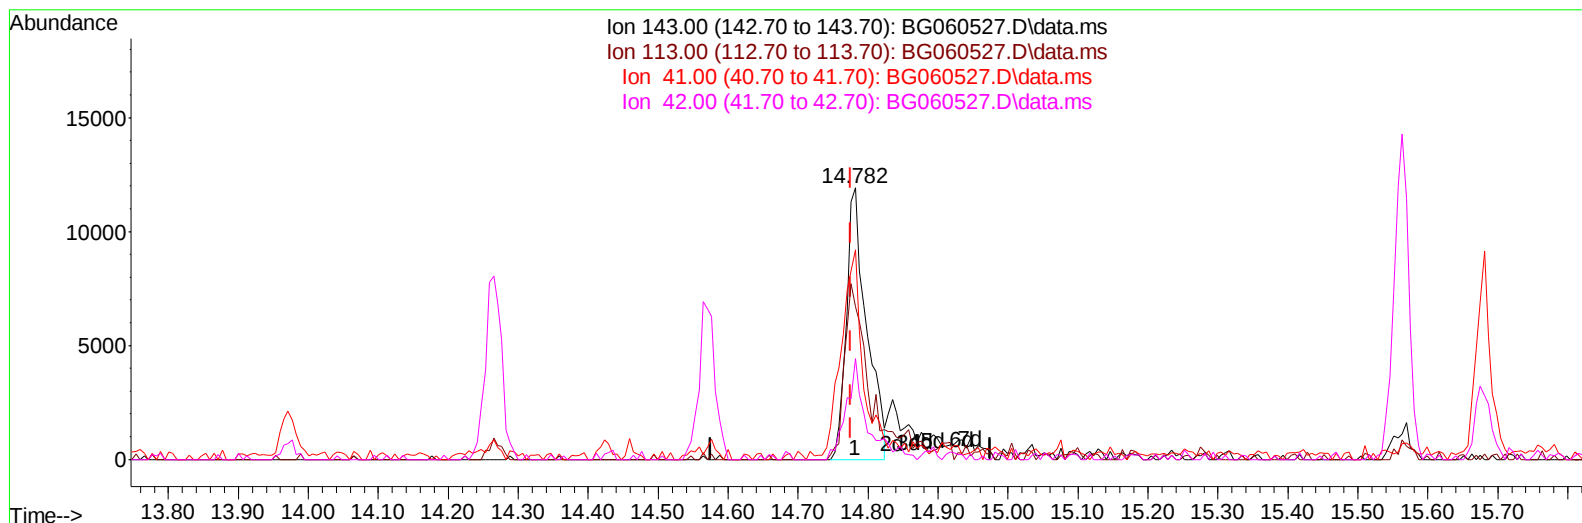

TIC: BG060527.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.782min (+ 0.007) 3.56 ng/ul

response 23985

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.60	56.31
41.00	29.80	77.17#
42.00	22.70	37.21#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
 Data File : BG060527.D
 Acq On : 1 Feb 2024 4:00
 Operator : MA/JU
 Sample : P1289-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 04:33:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 31 22:04:13 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/01/2024
 Supervised By :Sohil Jodhani 02/02/2024

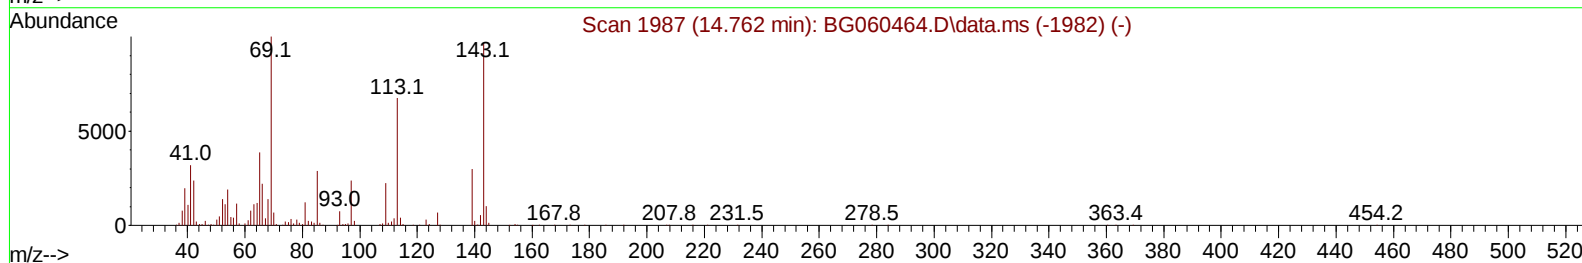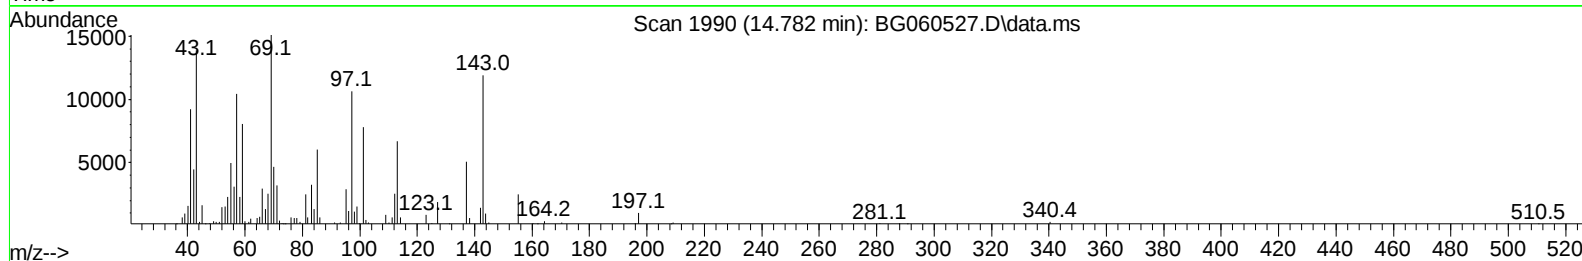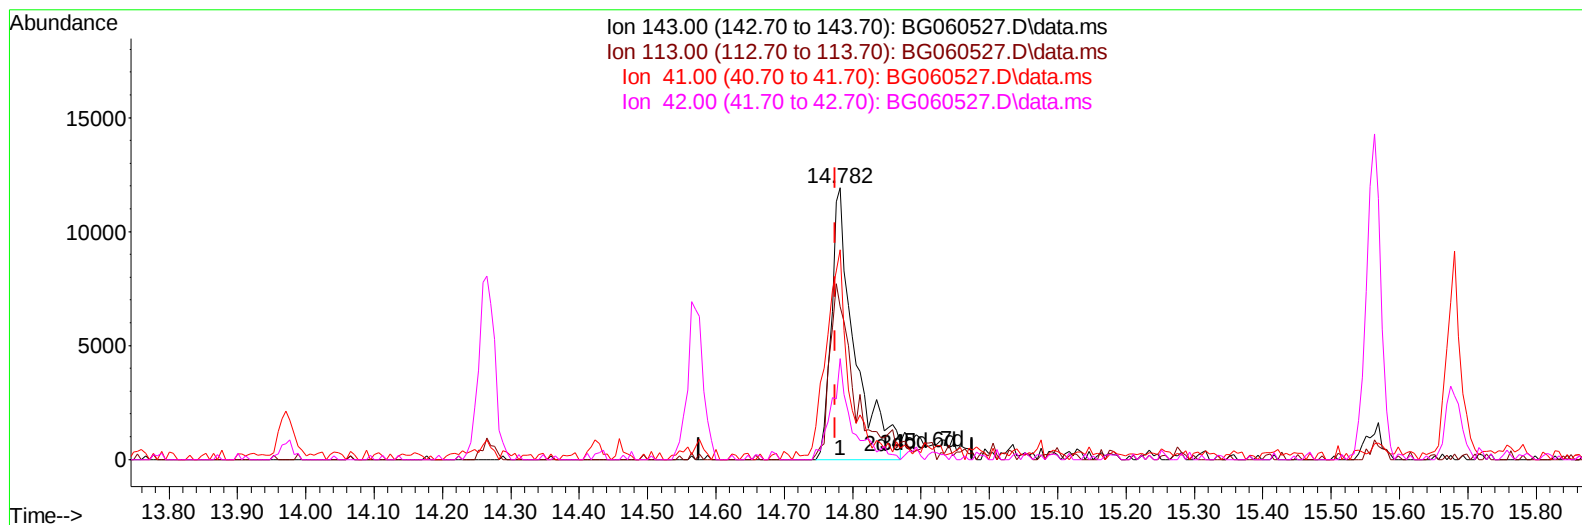

TIC: BG060527.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.782min (+ 0.007) 4.23 ng/ul m

response 28533

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.60	56.31
41.00	29.80	77.17#
42.00	22.70	37.21#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
 Data File : BG060527.D
 Acq On : 1 Feb 2024 4:00
 Operator : MA/JU
 Sample : P1289-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/01/2024
 Supervised By :Sohil Jodhani 02/02/2024

Quant Time: Feb 01 04:34:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 31 22:04:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.937	152	188662	20.000	ng/ul	0.00
20) Naphthalene-d8	10.739	136	759890	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.570	164	575341	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.320	188	1347433	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	1213581	20.000	ng/ul	0.00
88) Perylene-d12	24.752	264	1346023	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	16595	4.408	ng/uL	0.00
4) Pyridine-d5	3.783	84	83771	7.034	ng/ul	0.00
7) Phenol-d5	7.097	99	88793	4.956	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.261	67	313302	27.826	ng/ul	0.00
11) 2-Chlorophenol-d4	7.467	132	259719	21.706	ng/ul	0.00
15) 4-Methylphenol-d8	8.642	113	182962	12.397	ng/ul	0.00
21) Nitrobenzene-d5	9.094	128	186980	33.356	ng/ul	0.00
24) 2-Nitrophenol-d4	9.817	143	215807	32.952	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.358	165	394340	28.953	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	460819	25.791	ng/ul	0.00
46) Dimethylphthalate-d6	13.971	166	1504269	31.952	ng/ul	0.00
49) Acenaphthylene-d8	14.265	160	1707137	32.327	ng/ul	0.00
54) 4-Nitrophenol-d4	14.782	143	28533m	4.231	ng/ul	0.00
60) Fluorene-d10	15.563	176	1350158	32.730	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	234503	28.106	ng/ul	0.00
73) Anthracene-d10	17.414	188	2299648	36.003	ng/ul	0.00
81) Pyrene-d10	19.711	212	2667777	36.678	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.535	264	2661625	37.695	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060527.D
Acq On : 1 Feb 2024 4:00
Operator : MA/JU
Sample : P1289-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 04:34:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 31 22:04:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/01/2024
Supervised By :Sohil Jodhani 02/02/2024

