

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
 Data File : BG060512.D
 Acq On : 31 Jan 2024 17:14
 Operator : MA/JU
 Sample : PB158720BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK720

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG060512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.367	44	47	52	rBV	28847	42473	0.86%	0.102%
2	3.437	57	59	62	rVB4	7115	5145	0.10%	0.012%
3	3.784	113	118	131	rBV	361110	646386	13.14%	1.545%
4	4.124	172	176	180	rVB2	5165	9115	0.19%	0.022%
5	4.436	223	229	231	rBV6	5579	10876	0.22%	0.026%
6	6.222	530	533	536	rVB4	3354	5152	0.10%	0.012%
7	6.257	536	539	542	rBV3	5024	5581	0.11%	0.013%
8	6.639	600	604	607	rVB6	3770	5010	0.10%	0.012%
9	7.097	673	682	691	rBV	401053	735201	14.95%	1.757%
10	7.262	703	710	721	rBV	298671	514187	10.46%	1.229%
11	7.468	738	745	761	rBV	328706	605584	12.31%	1.447%
12	7.932	816	824	836	rBV	325965	598357	12.17%	1.430%
13	8.637	938	944	960	rBV	459013	884373	17.98%	2.113%
14	9.095	1015	1022	1035	rBV	363352	675042	13.73%	1.613%
15	9.818	1139	1145	1158	rVV2	301560	566645	11.52%	1.354%
16	10.358	1229	1237	1251	rBV	474047	927313	18.86%	2.216%
17	10.734	1293	1301	1312	rBV	537116	1000968	20.35%	2.392%
18	10.875	1317	1325	1336	rBV	467433	944555	19.21%	2.257%
19	12.333	1568	1573	1577	rBV3	7031	12988	0.26%	0.031%
20	13.461	1758	1765	1771	rBV4	10023	21268	0.43%	0.051%
21	13.972	1845	1852	1865	rBV	1232098	1846656	37.55%	4.413%
22	14.266	1892	1902	1915	rBV	1384155	2208737	44.91%	5.278%
23	14.571	1945	1954	1964	rBV	1161492	1812029	36.85%	4.330%
24	14.647	1964	1967	1970	rVB3	4298	6491	0.13%	0.016%
25	14.771	1982	1988	2003	rBV	355864	703230	14.30%	1.681%
26	15.564	2116	2123	2134	rBV	1952887	2998256	60.97%	7.165%
27	15.682	2137	2143	2152	rBV	502320	759125	15.44%	1.814%
28	15.805	2161	2164	2167	rVB5	10212	10072	0.20%	0.024%
29	16.134	2215	2220	2223	rBV5	4031	7259	0.15%	0.017%
30	16.334	2251	2254	2256	rBV3	10305	12291	0.25%	0.029%
31	17.074	2376	2380	2382	rBV3	6505	6813	0.14%	0.016%
32	17.109	2382	2386	2389	rBV	6190	9702	0.20%	0.023%
33	17.321	2413	2422	2431	rBV	1731681	2694315	54.79%	6.439%
34	17.415	2431	2438	2451	rVV	2487025	3717380	75.59%	8.884%
35	18.055	2544	2547	2549	rVV4	4651	5041	0.10%	0.012%
36	18.408	2603	2607	2608	rBV3	4043	5144	0.10%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060512.D
Acq On : 31 Jan 2024 17:14
Operator : MA/JU
Sample : PB158720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK720

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Title : SVOA CALIBRATION

37	19.013	2708	2710	2715	rVB6	4441	6049	0.12%	0.014%
38	19.148	2731	2733	2737	rVB5	4635	5728	0.12%	0.014%
39	19.271	2748	2754	2761	rVB3	41580	71806	1.46%	0.172%
40	19.348	2761	2767	2772	rBV	38245	70038	1.42%	0.167%
41	19.471	2784	2788	2790	rVV5	4455	6973	0.14%	0.017%
42	19.583	2803	2807	2808	rBV4	6981	8752	0.18%	0.021%
43	19.624	2810	2814	2818	rVB7	12640	15520	0.32%	0.037%
44	19.712	2822	2829	2839	rBV	3349448	4917752	100.00%	11.752%
45	20.153	2902	2904	2906	rBV3	7820	6284	0.13%	0.015%
46	20.623	2982	2984	2985	rBV2	12162	9878	0.20%	0.024%
47	21.580	3140	3147	3156	rBV2	1969465	3223911	65.56%	7.704%
48	23.038	3390	3395	3400	rBV6	35322	79331	1.61%	0.190%
49	24.536	3637	3650	3664	rBV2	1744741	4879801	99.23%	11.662%
50	24.753	3675	3687	3702	rBV	1236248	3524120	71.66%	8.422%




Sum of corrected areas: 41844703

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060512.D
Acq On : 31 Jan 2024 17:14
Operator : MA/JU
Sample : PB158720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK720

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

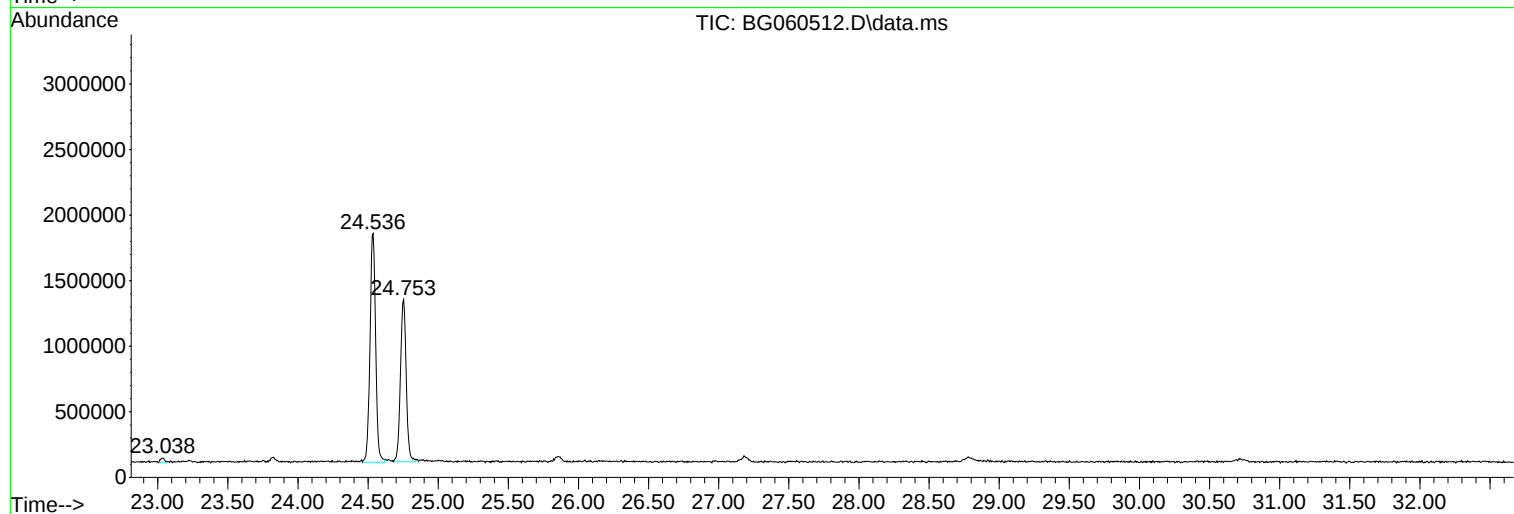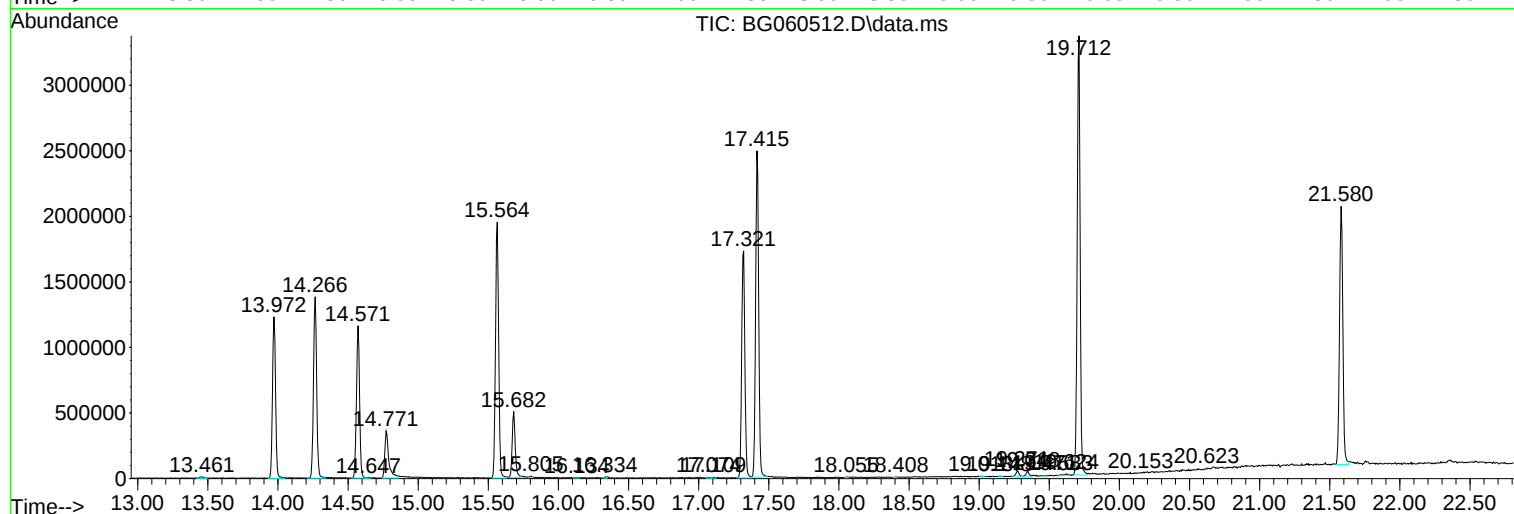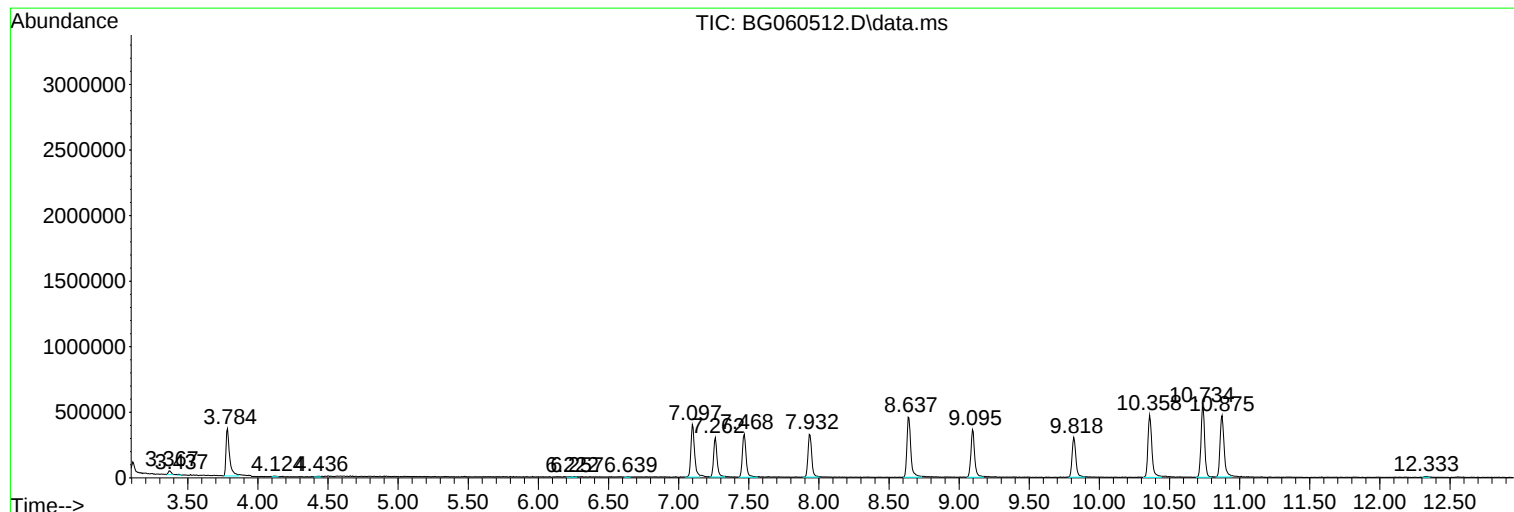

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060512.D
Acq On : 31 Jan 2024 17:14
Operator : MA/JU
Sample : PB158720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK720

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060512.D
Acq On : 31 Jan 2024 17:14
Operator : MA/JU
Sample : PB158720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK720

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc