

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
 Data File : BG060515.D
 Acq On : 31 Jan 2024 19:15
 Operator : MA/JU
 Sample : P1289-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG060515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.347	41	44	46	rBV4	12367	16202	0.24%	0.030%
2	3.371	46	48	50	rVV3	22608	19500	0.29%	0.036%
3	3.406	50	54	60	rVB	27681	43751	0.64%	0.081%
4	3.788	116	119	126	rBV	70475	114113	1.68%	0.212%
5	4.111	172	174	179	rVB4	8007	10561	0.16%	0.020%
6	5.039	329	332	336	rBV4	9982	12623	0.19%	0.023%
7	7.102	678	683	695	rBV	90505	183842	2.71%	0.342%
8	7.260	704	710	721	rBV	395266	715458	10.54%	1.329%
9	7.466	738	745	758	rBV2	328500	610115	8.99%	1.134%
10	7.936	818	825	836	rBV	401244	740677	10.91%	1.376%
11	8.053	841	845	850	rVB6	15375	24495	0.36%	0.046%
12	8.641	937	945	963	rBV2	278781	579778	8.54%	1.077%
13	9.093	1016	1022	1037	rBV	538104	988414	14.56%	1.836%
14	9.816	1138	1145	1159	rBV	421202	809589	11.92%	1.504%
15	10.357	1230	1237	1256	rBV	646666	1274439	18.77%	2.368%
16	10.739	1295	1302	1312	rBV	712258	1285699	18.94%	2.389%
17	10.874	1317	1325	1334	rBV	575118	1133044	16.69%	2.105%
18	11.491	1426	1430	1433	rBV3	5731	7249	0.11%	0.013%
19	11.984	1510	1514	1519	rVB3	9172	16129	0.24%	0.030%
20	12.325	1567	1572	1577	rBV3	11578	23726	0.35%	0.044%
21	13.453	1760	1764	1771	rVB	27600	43326	0.64%	0.080%
22	13.970	1844	1852	1861	rBV	1749508	2648032	39.00%	4.920%
23	14.264	1895	1902	1913	rBV	2184490	3364219	49.55%	6.250%
24	14.569	1946	1954	1964	rBV	1606617	2437782	35.90%	4.529%
25	14.787	1985	1991	1999	rBV2	52178	125282	1.85%	0.233%
26	15.404	2093	2096	2103	rVB4	3277	7744	0.11%	0.014%
27	15.562	2115	2123	2137	rBV	3019243	4594058	67.66%	8.535%
28	15.680	2137	2143	2154	rVV	699286	1065251	15.69%	1.979%
29	15.803	2161	2164	2168	rVB4	19417	23508	0.35%	0.044%
30	16.350	2253	2257	2261	rVB5	12317	17092	0.25%	0.032%
31	16.996	2365	2367	2373	rVB6	6628	9404	0.14%	0.017%
32	17.319	2415	2422	2432	rBV	2283438	3369352	49.62%	6.260%
33	17.419	2432	2439	2452	rVV	3573913	5463044	80.46%	10.150%
34	17.977	2531	2534	2536	rBV4	8012	8793	0.13%	0.016%
35	18.206	2571	2573	2576	rVV3	6180	7640	0.11%	0.014%
36	18.277	2582	2585	2589	rBV6	7133	8357	0.12%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060515.D
Acq On : 31 Jan 2024 19:15
Operator : MA/JU
Sample : P1289-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Title : SVOA CALIBRATION

37	18.706	2654	2658	2661	rBV5	5427	8344	0.12%	0.016%
38	19.117	2726	2728	2732	rBV5	6477	7925	0.12%	0.015%
39	19.270	2749	2754	2760	rBV2	59783	89671	1.32%	0.167%
40	19.340	2762	2766	2771	rBV	46771	70185	1.03%	0.130%
41	19.616	2810	2813	2820	rBV7	20344	26261	0.39%	0.049%
42	19.710	2822	2829	2841	rBV	4636381	6789732	100.00%	12.615%
43	19.934	2865	2867	2871	rVB3	13473	13371	0.20%	0.025%
44	20.239	2915	2919	2920	rBV3	8803	10873	0.16%	0.020%
45	20.668	2989	2992	2994	rBV4	20754	23349	0.34%	0.043%
46	20.727	2999	3002	3005	rBV5	16234	20599	0.30%	0.038%
47	21.226	3084	3087	3090	rBV5	38764	52681	0.78%	0.098%
48	21.579	3141	3147	3159	rBV2	2261504	3791556	55.84%	7.044%
49	21.896	3199	3201	3203	rBV3	16168	16583	0.24%	0.031%
50	23.224	3422	3427	3432	rVB	62355	103765	1.53%	0.193%
51	23.635	3495	3497	3499	rBV3	14847	11025	0.16%	0.020%
52	23.823	3525	3529	3534	rVB3	60036	107893	1.59%	0.200%
53	24.534	3639	3650	3663	rBV2	2437815	6683414	98.43%	12.417%
54	24.752	3677	3687	3699	rVB2	1431134	3999357	58.90%	7.431%
55	25.457	3805	3807	3808	rBV2	16536	10350	0.15%	0.019%
56	25.850	3870	3874	3885	rVB4	67609	170968	2.52%	0.318%
57	28.712	4359	4361	4362	rBV2	18027	13121	0.19%	0.024%




Sum of corrected areas: 53823311

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060515.D
Acq On : 31 Jan 2024 19:15
Operator : MA/JU
Sample : P1289-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

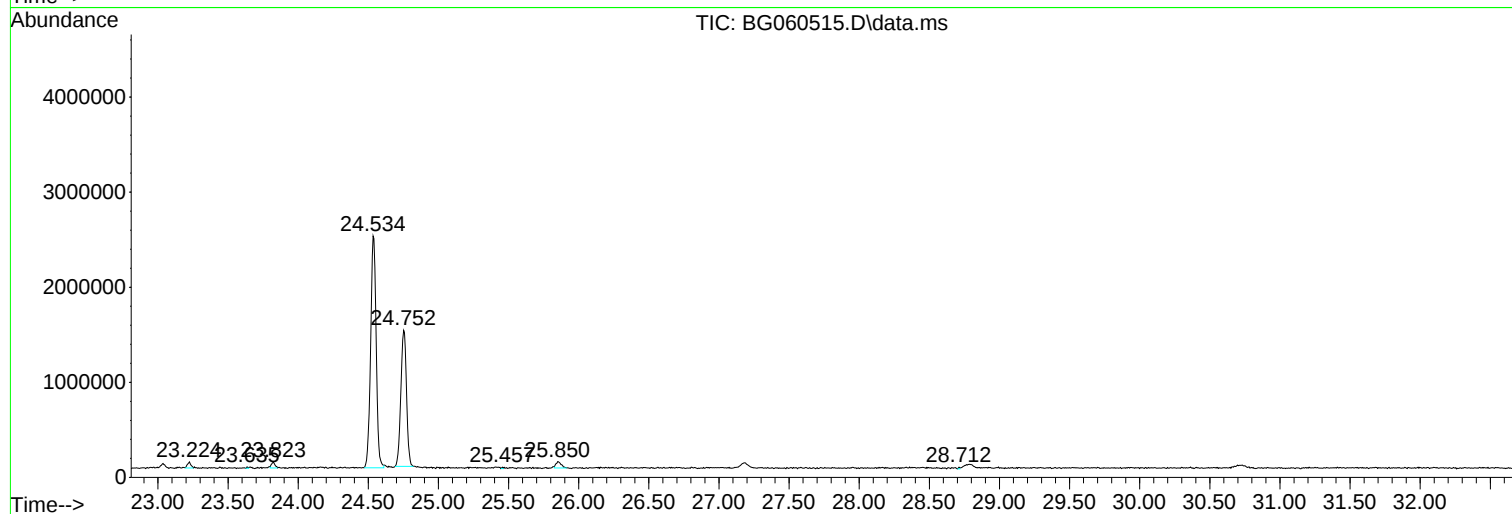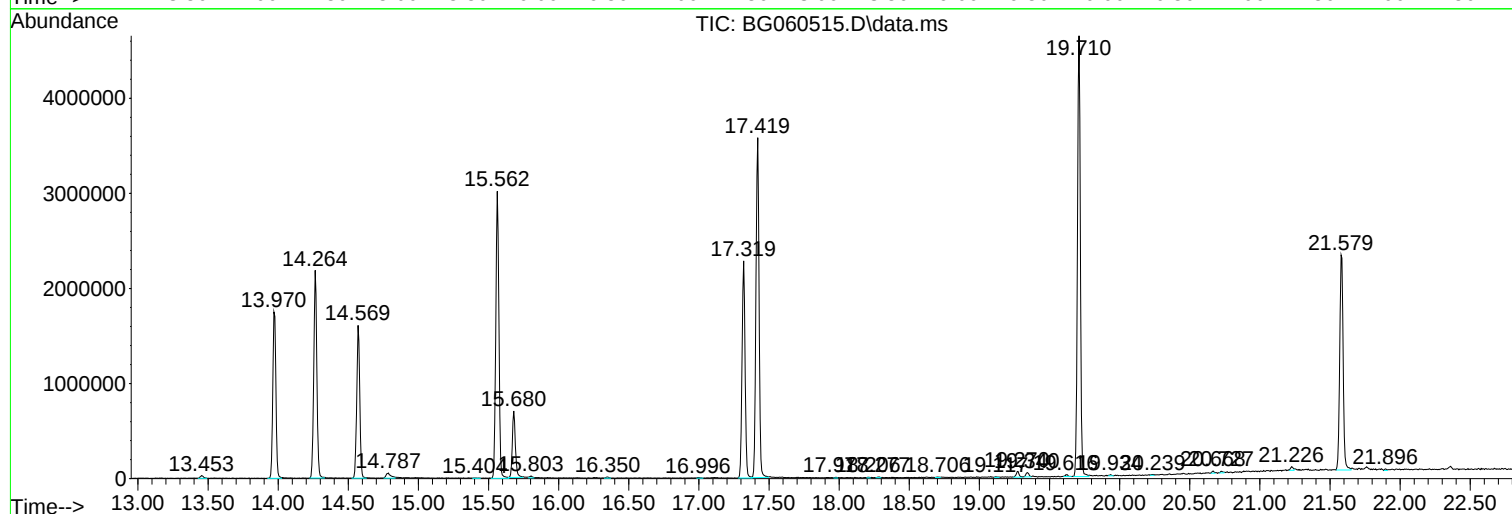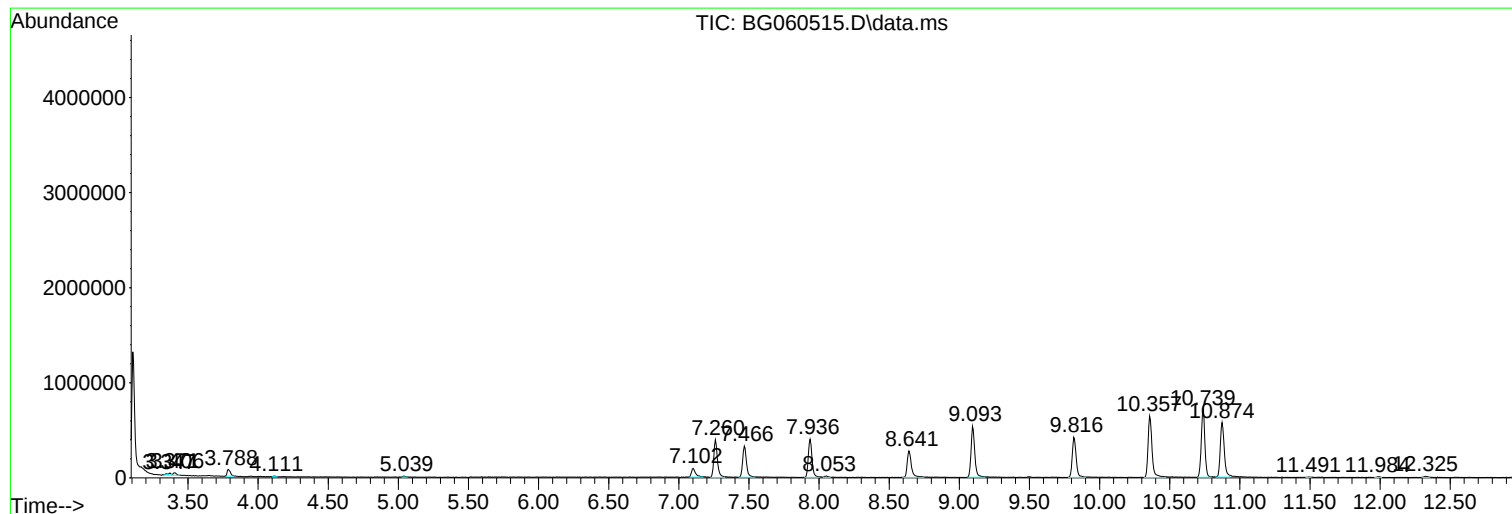

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060515.D
Acq On : 31 Jan 2024 19:15
Operator : MA/JU
Sample : P1289-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060515.D
Acq On : 31 Jan 2024 19:15
Operator : MA/JU
Sample : P1289-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
