

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
 Data File : BG060522.D
 Acq On : 31 Jan 2024 23:57
 Operator : MA/JU
 Sample : P1289-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG060522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	43	47	52	rBV3	18160	29556	0.43%	0.060%
2	3.787	115	119	128	rBV	37527	71821	1.04%	0.145%
3	4.122	171	176	179	rBV4	6970	12033	0.17%	0.024%
4	4.275	200	202	205	rVB4	6050	7024	0.10%	0.014%
5	5.039	327	332	337	rVB4	12945	19686	0.29%	0.040%
6	7.101	677	683	696	rBV2	75804	157824	2.29%	0.319%
7	7.260	703	710	723	rBV	389136	696771	10.11%	1.408%
8	7.465	739	745	758	rBV	308405	580094	8.42%	1.172%
9	7.935	819	825	838	rBV	349408	635790	9.23%	1.284%
10	8.640	938	945	962	rBV	272666	516143	7.49%	1.043%
11	9.093	1016	1022	1034	rBV	479147	914818	13.28%	1.848%
12	9.492	1085	1090	1095	rBV3	13721	23884	0.35%	0.048%
13	9.815	1139	1145	1159	rBV	376109	701779	10.19%	1.418%
14	10.356	1230	1237	1250	rBV	580242	1118188	16.23%	2.259%
15	10.738	1294	1302	1314	rBV	566934	1050489	15.25%	2.122%
16	10.873	1318	1325	1337	rBV	401190	783772	11.38%	1.583%
17	11.989	1512	1515	1521	rBV4	11546	16912	0.25%	0.034%
18	12.318	1567	1571	1578	rBV3	12955	24254	0.35%	0.049%
19	13.382	1748	1752	1757	rVB5	6569	10145	0.15%	0.020%
20	13.458	1757	1765	1771	rBV3	18912	36862	0.54%	0.074%
21	13.975	1845	1853	1860	rBV	1632620	2396467	34.78%	4.841%
22	14.263	1895	1902	1913	rBV	1944425	3043573	44.18%	6.149%
23	14.569	1944	1954	1966	rBV	1179452	1894498	27.50%	3.827%
24	14.774	1984	1989	2000	rBV4	59832	149717	2.17%	0.302%
25	15.350	2083	2087	2092	rBV7	4175	8541	0.12%	0.017%
26	15.562	2117	2123	2136	rBV	2870134	4210199	61.11%	8.505%
27	15.679	2137	2143	2159	rVV	708206	1105827	16.05%	2.234%
28	15.803	2159	2164	2170	rVB8	16095	27976	0.41%	0.057%
29	16.132	2215	2220	2223	rBV5	5782	11097	0.16%	0.022%
30	16.267	2240	2243	2248	rVB5	7493	9713	0.14%	0.020%
31	16.343	2251	2256	2260	rVV5	11996	16138	0.23%	0.033%
32	16.989	2364	2366	2370	rBV3	6234	8200	0.12%	0.017%
33	17.318	2414	2422	2432	rBV	1824293	2758136	40.03%	5.572%
34	17.418	2432	2439	2453	rVB2	3442041	5298427	76.91%	10.704%
35	17.700	2484	2487	2493	rVB7	6273	8677	0.13%	0.018%
36	17.982	2530	2535	2538	rVB5	11175	16973	0.25%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
 Data File : BG060522.D
 Acq On : 31 Jan 2024 23:57
 Operator : MA/JU
 Sample : P1289-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Title : SVOA CALIBRATION

37	18.200	2570	2572	2578	rBV6	13929	19854	0.29%	0.040%
38	18.270	2581	2584	2590	rVB4	8270	13036	0.19%	0.026%
39	18.629	2640	2645	2648	rBV5	17813	25731	0.37%	0.052%
40	19.210	2739	2744	2745	rBV5	7448	9312	0.14%	0.019%
41	19.275	2750	2755	2759	rBV3	58133	92692	1.35%	0.187%
42	19.345	2763	2767	2771	rVV	46904	66076	0.96%	0.133%
43	19.580	2806	2807	2810	rBV3	6307	6936	0.10%	0.014%
44	19.622	2810	2814	2817	rVV4	22211	24247	0.35%	0.049%
45	19.710	2822	2829	2841	rVV	4802145	6731057	97.70%	13.598%
46	19.898	2858	2861	2864	rBV5	5785	9086	0.13%	0.018%
47	20.662	2989	2991	2997	rVB7	18666	23602	0.34%	0.048%
48	21.226	3082	3087	3094	rBV5	60575	121371	1.76%	0.245%
49	21.461	3124	3127	3131	rBV2	29495	40364	0.59%	0.082%
50	21.578	3140	3147	3158	rBV	1861600	3125747	45.37%	6.315%
51	21.931	3205	3207	3210	rBV4	11622	11596	0.17%	0.023%
52	22.354	3277	3279	3284	rVB4	26036	33121	0.48%	0.067%
53	23.029	3389	3394	3402	rVB7	46807	106887	1.55%	0.216%
54	23.217	3423	3426	3434	rVB2	49644	84829	1.23%	0.171%
55	23.823	3525	3529	3534	rVB5	55111	103613	1.50%	0.209%
56	24.533	3638	3650	3667	rBV2	2471996	6889371	100.00%	13.918%
57	24.751	3676	3687	3700	rVB2	1206199	3391384	49.23%	6.851%
58	25.844	3868	3873	3883	rVB6	50696	157262	2.28%	0.318%
59	26.226	3935	3938	3939	rBV3	16247	15030	0.22%	0.030%
60	26.995	4067	4069	4073	rBV5	14065	15987	0.23%	0.032%
61	28.864	4385	4387	4388	rVB	17600	10200	0.15%	0.021%




Sum of corrected areas: 49500395

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060522.D
Acq On : 31 Jan 2024 23:57
Operator : MA/JU
Sample : P1289-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

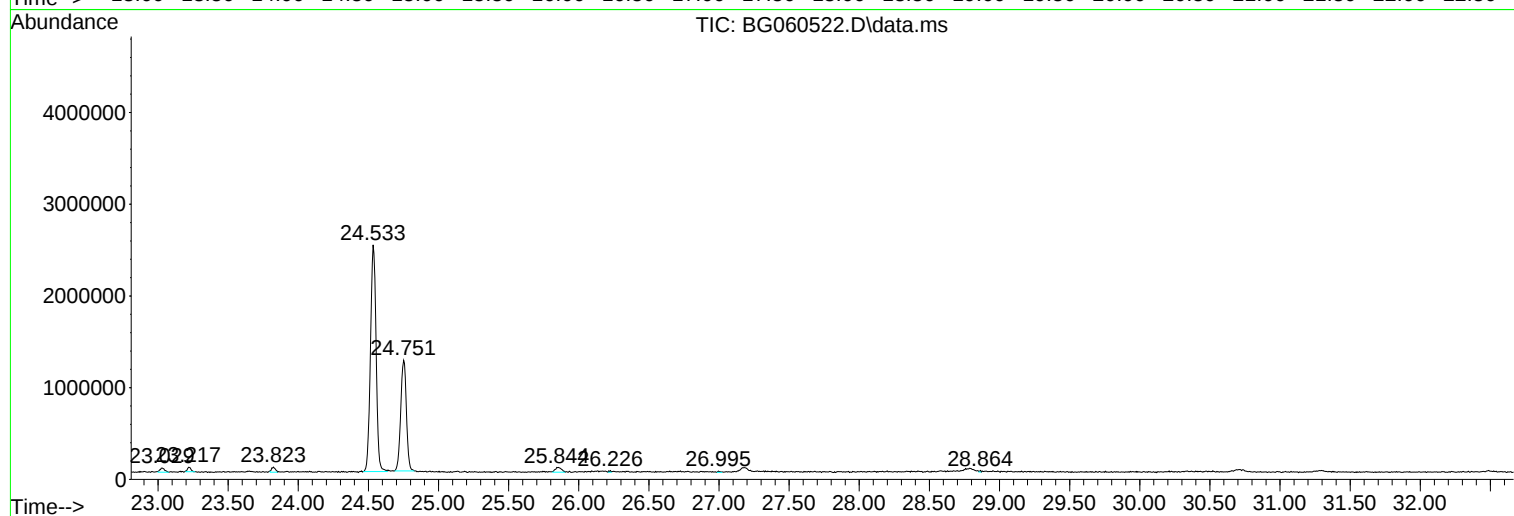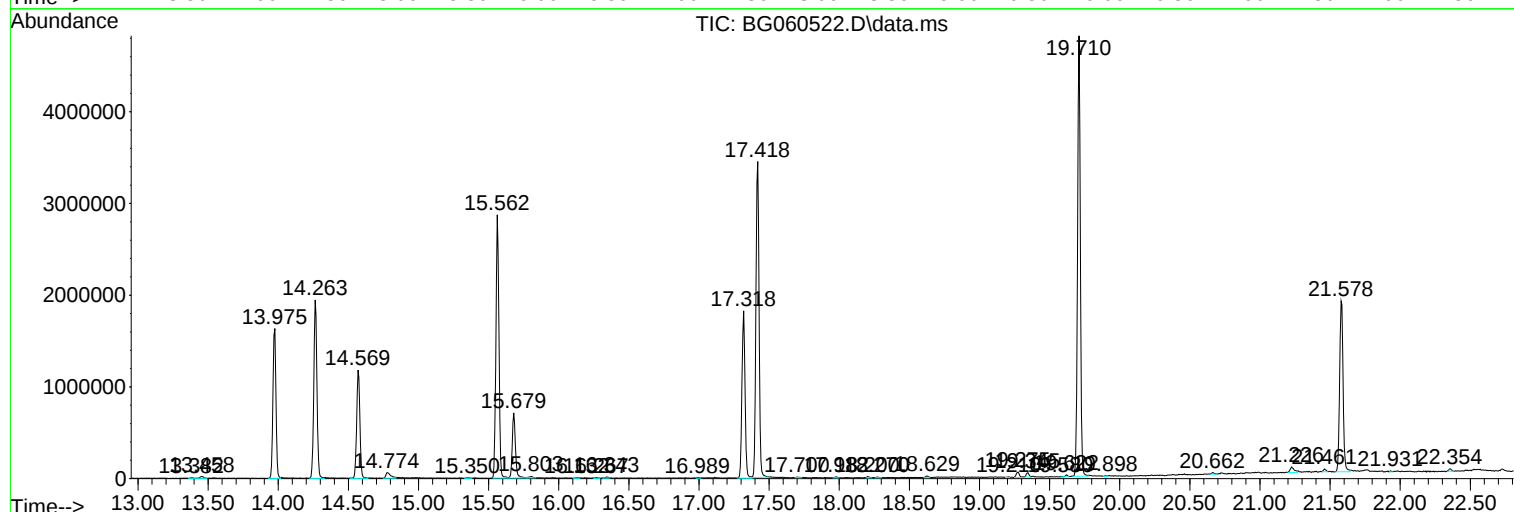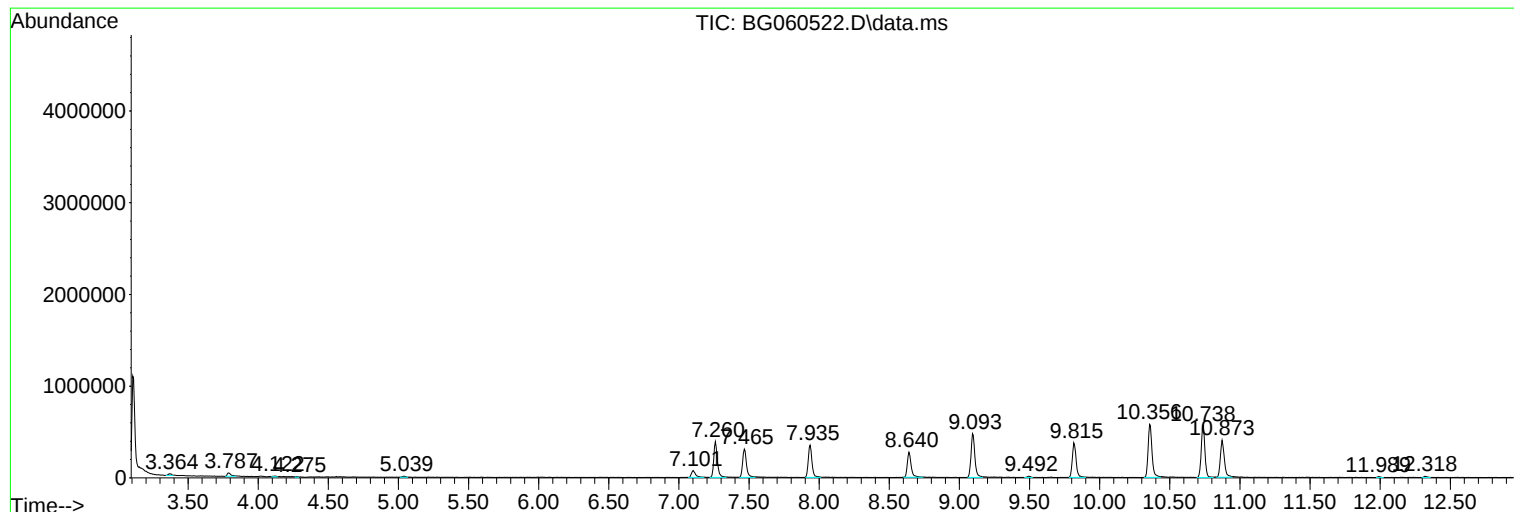

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060522.D
Acq On : 31 Jan 2024 23:57
Operator : MA/JU
Sample : P1289-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060522.D
Acq On : 31 Jan 2024 23:57
Operator : MA/JU
Sample : P1289-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc