

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060526.D
Acq On : 1 Feb 2024 3:19
Operator : MA/JU
Sample : PB158739BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK739

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BG060526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.172	13	14	17	rBV3	10060	9941	0.20%	0.023%
2	3.372	44	48	53	rVB2	32429	39907	0.79%	0.092%
3	3.560	79	80	85	rBV3	4956	6873	0.14%	0.016%
4	3.783	113	118	135	rBV	289755	527648	10.39%	1.222%
5	4.118	171	175	183	rVB5	8026	15414	0.30%	0.036%
6	4.436	226	229	234	rBV4	2903	5952	0.12%	0.014%
7	4.512	238	242	246	rBV4	3952	6780	0.13%	0.016%
8	7.097	675	682	698	rBV	365285	723994	14.26%	1.677%
9	7.262	703	710	726	rVV	320904	581332	11.45%	1.347%
10	7.467	737	745	757	rBV	341644	670066	13.20%	1.552%
11	7.597	765	767	771	rVB5	3758	5193	0.10%	0.012%
12	7.937	818	825	835	rBV	296061	550936	10.85%	1.276%
13	8.642	937	945	958	rBV	494341	950460	18.72%	2.202%
14	9.095	1015	1022	1037	rBV	380399	743306	14.64%	1.722%
15	9.224	1041	1044	1051	rBV5	4554	6149	0.12%	0.014%
16	9.817	1138	1145	1156	rBV	323173	618618	12.18%	1.433%
17	10.358	1229	1237	1253	rBV	528843	1074350	21.16%	2.489%
18	10.740	1294	1302	1314	rBV	483421	894445	17.62%	2.072%
19	10.875	1318	1325	1339	rBV	513658	1060269	20.88%	2.456%
20	12.320	1569	1571	1580	rVB4	10399	18289	0.36%	0.042%
21	12.867	1663	1664	1671	rVB2	2850	5903	0.12%	0.014%
22	13.454	1760	1764	1769	rBV3	14835	24728	0.49%	0.057%
23	13.543	1776	1779	1784	rVB6	5126	7052	0.14%	0.016%
24	13.971	1845	1852	1862	rBV	1367475	1991850	39.23%	4.614%
25	14.265	1894	1902	1913	rBV	1558475	2474438	48.73%	5.733%
26	14.347	1913	1916	1920	rVB3	4947	7754	0.15%	0.018%
27	14.571	1945	1954	1964	rBV	1102210	1687311	33.23%	3.909%
28	14.770	1983	1988	1999	rBV2	381961	758179	14.93%	1.756%
29	15.564	2116	2123	2136	rBV	2236277	3402550	67.01%	7.883%
30	15.681	2137	2143	2150	rBV	504693	779376	15.35%	1.806%
31	15.799	2160	2163	2172	rVB6	12933	24274	0.48%	0.056%
32	16.345	2250	2256	2263	rBV5	10942	20206	0.40%	0.047%
33	16.997	2362	2367	2370	rVB5	5346	8473	0.17%	0.020%
34	17.320	2414	2422	2431	rBV	1540710	2442039	48.09%	5.657%
35	17.420	2432	2439	2450	rVV	2628065	4041705	79.60%	9.363%
36	17.837	2503	2510	2513	rBV3	2664	5898	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
 Data File : BG060526.D
 Acq On : 1 Feb 2024 3:19
 Operator : MA/JU
 Sample : PB158739BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK739

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
 Title : SVOA CALIBRATION

37	18.172	2562	2567	2568	rVB3	3983	5992	0.12%	0.014%
38	18.225	2575	2576	2579	rBV2	4745	5519	0.11%	0.013%
39	18.507	2622	2624	2628	rBV3	4201	6048	0.12%	0.014%
40	18.719	2657	2660	2663	rVB4	5131	7310	0.14%	0.017%
41	19.271	2749	2754	2761	rBV	41473	66438	1.31%	0.154%
42	19.342	2761	2766	2771	rBV3	35725	57670	1.14%	0.134%
43	19.624	2812	2814	2817	rBV3	13822	13167	0.26%	0.031%
44	19.706	2822	2828	2841	rVV	3472054	5077625	100.00%	11.763%
45	19.859	2852	2854	2857	rBV4	6589	8853	0.17%	0.021%
46	20.387	2942	2944	2947	rBV4	6468	7576	0.15%	0.018%
47	20.564	2972	2974	2976	rBV3	9152	9279	0.18%	0.021%
48	20.799	3012	3014	3019	rBV6	7294	11882	0.23%	0.028%
49	21.398	3114	3116	3117	rBV2	9995	5595	0.11%	0.013%
50	21.580	3140	3147	3156	rBV2	1688686	2779083	54.73%	6.438%
51	22.761	3346	3348	3352	rVB4	14816	14300	0.28%	0.033%
52	23.031	3390	3394	3400	rVB3	48032	90514	1.78%	0.210%
53	23.108	3405	3407	3409	rBV3	10968	8344	0.16%	0.019%
54	23.825	3523	3529	3536	rVB4	64623	148578	2.93%	0.344%
55	24.536	3639	3650	3663	rBV2	1768813	5018976	98.84%	11.627%
56	24.747	3676	3686	3700	rBV	1143975	3129054	61.62%	7.249%
57	25.852	3870	3874	3886	rVB3	78654	218081	4.29%	0.505%
58	27.191	4093	4102	4113	rVB6	74140	276578	5.45%	0.641%
59	31.322	4803	4805	4806	rBV2	12748	6946	0.14%	0.016%




Sum of corrected areas: 43165066

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060526.D
Acq On : 1 Feb 2024 3:19
Operator : MA/JU
Sample : PB158739BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK739

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

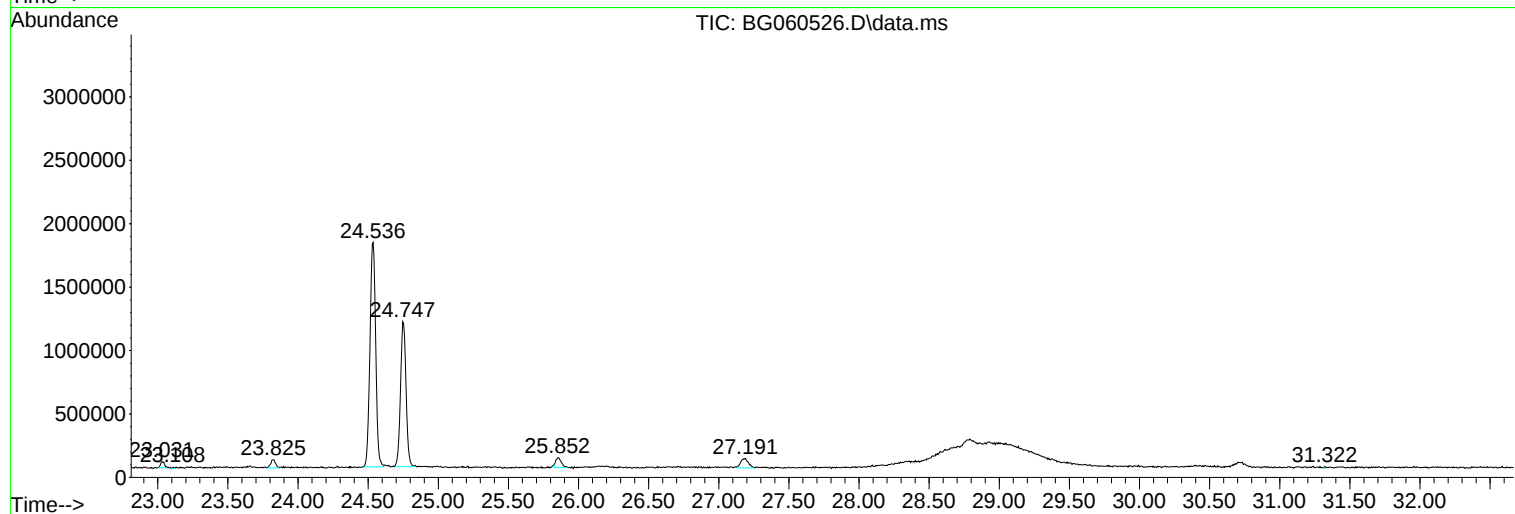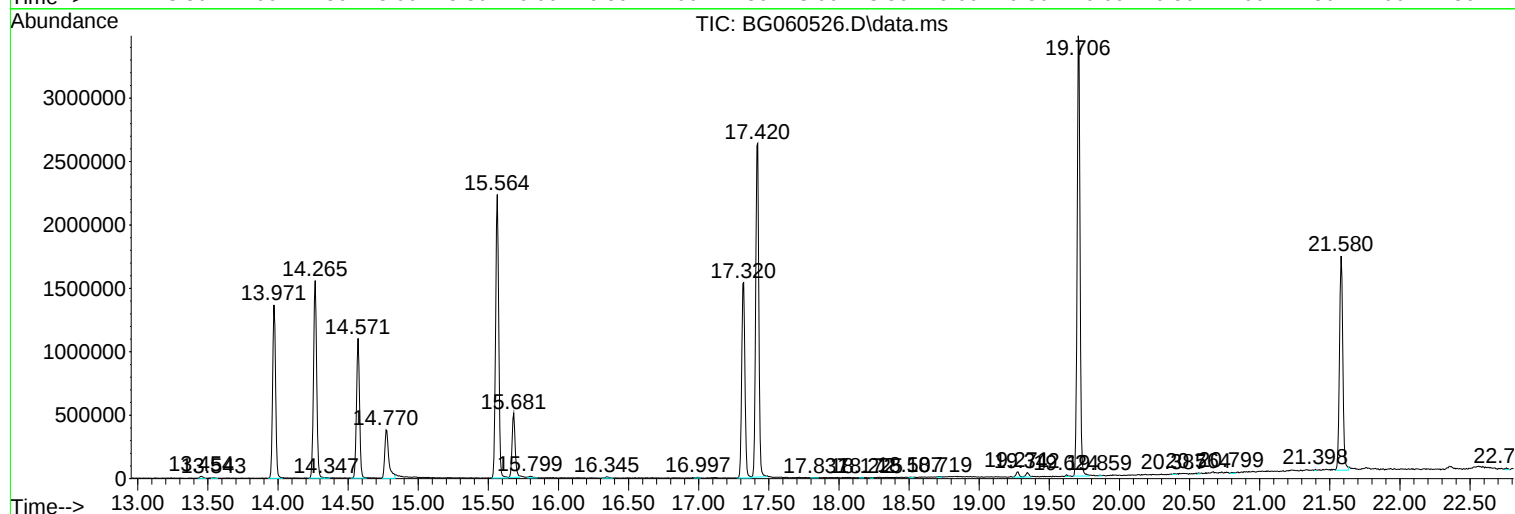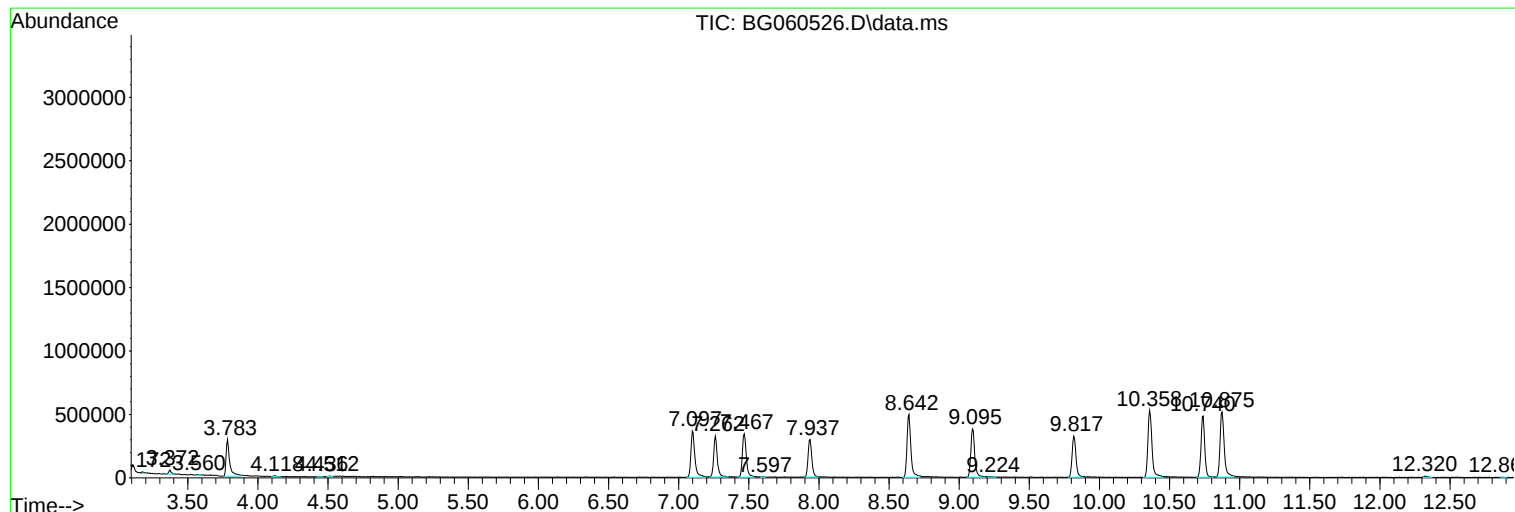

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060526.D
Acq On : 1 Feb 2024 3:19
Operator : MA/JU
Sample : PB158739BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK739

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020124\
Data File : BG060526.D
Acq On : 1 Feb 2024 3:19
Operator : MA/JU
Sample : PB158739BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK739

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG012624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc