
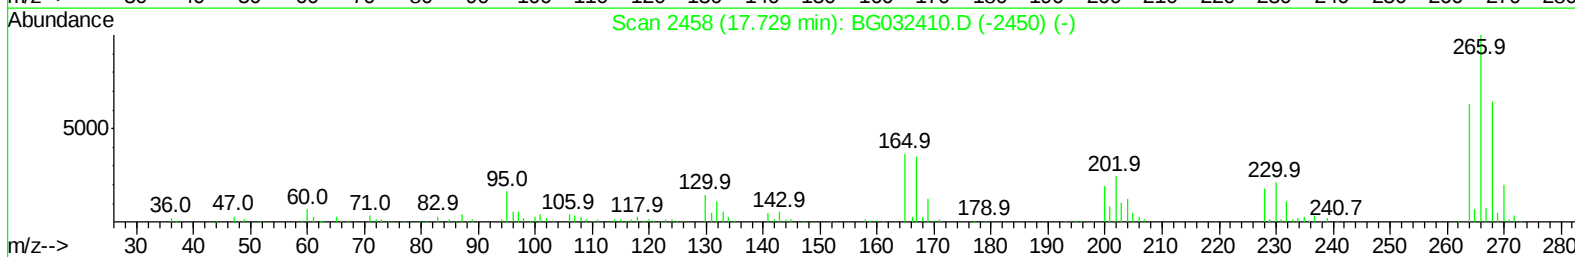
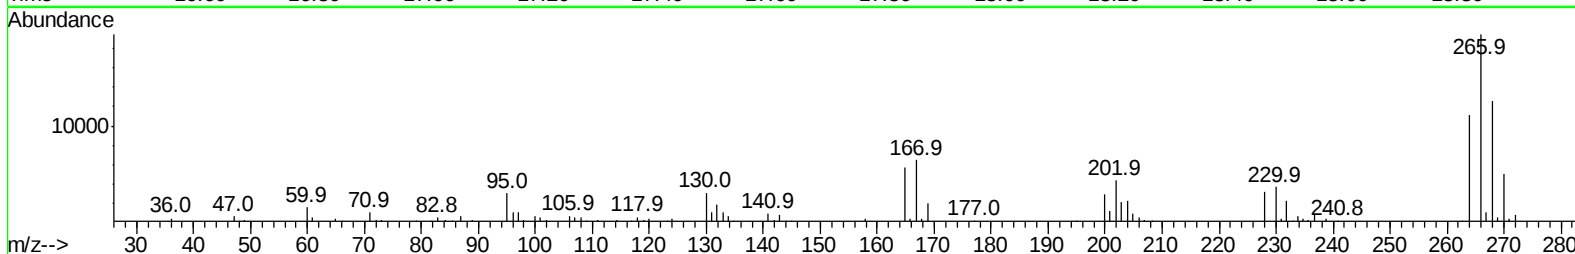


Data Path : U:\HPCHEM1\BNA G\DATA\BG020218\
Data File : BG032506.D
Acq On : 2 Feb 2018 10:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 00:10:02 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

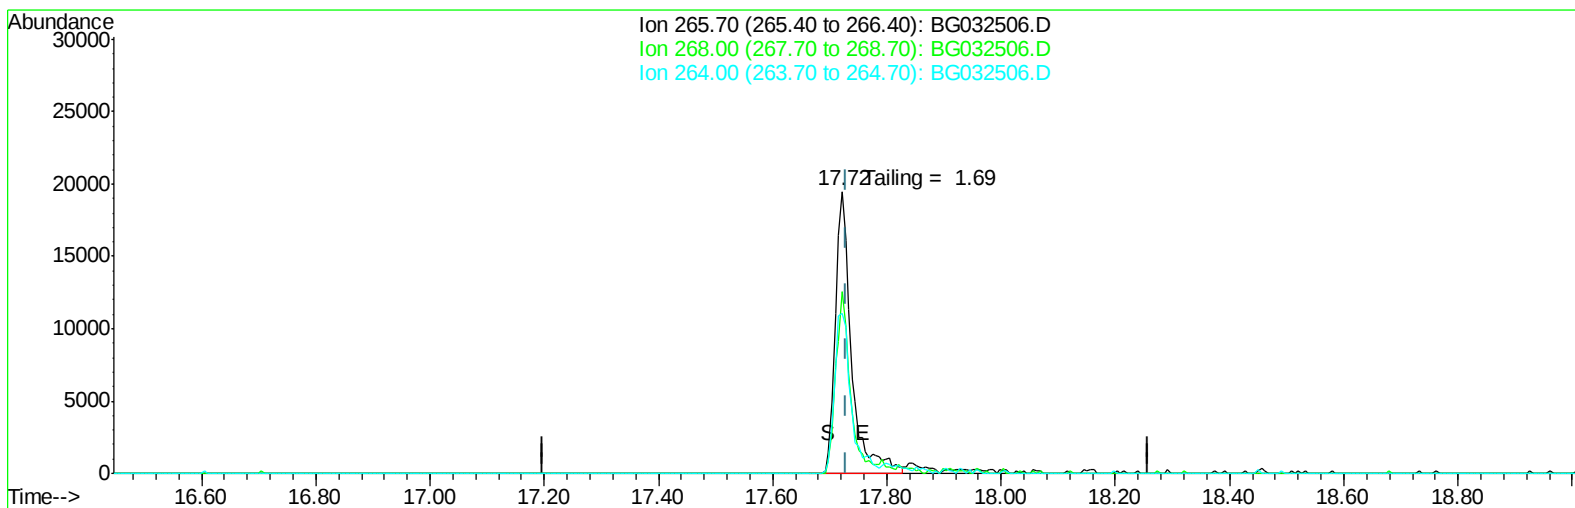

TIC: BG032506.D

(69) Pentachlorophenol (C)




17.721min (-0.007) 27570.73ng

response 38227

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.77
264.00	62.00	56.91
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG020218\
 Data File : BG032506.D
 Acq On : 2 Feb 2018 10:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 00:10:02 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 29 15:32:55 2018
 Response via : Initial Calibration

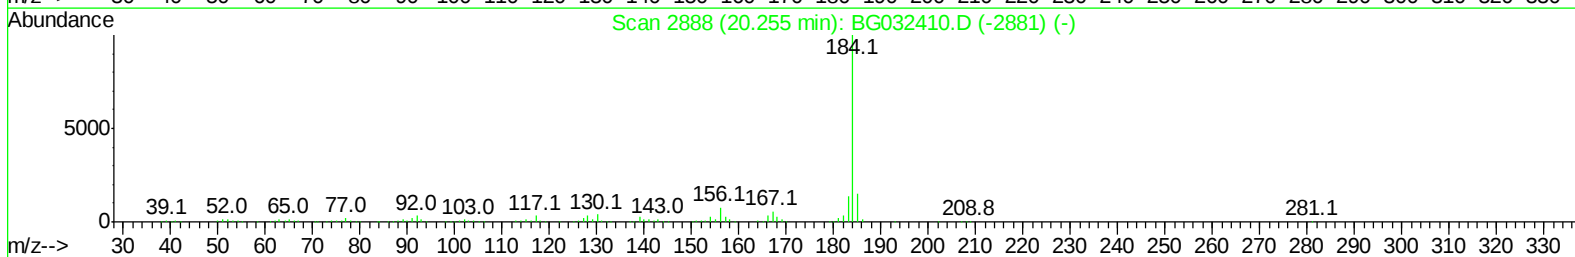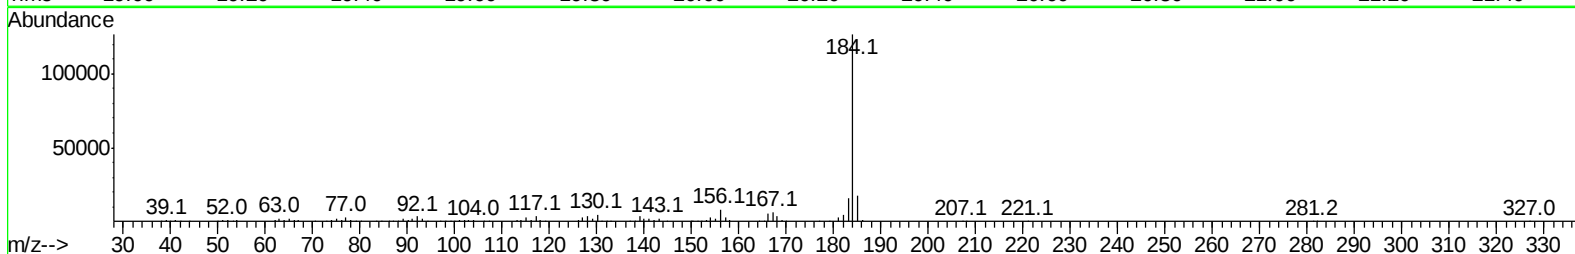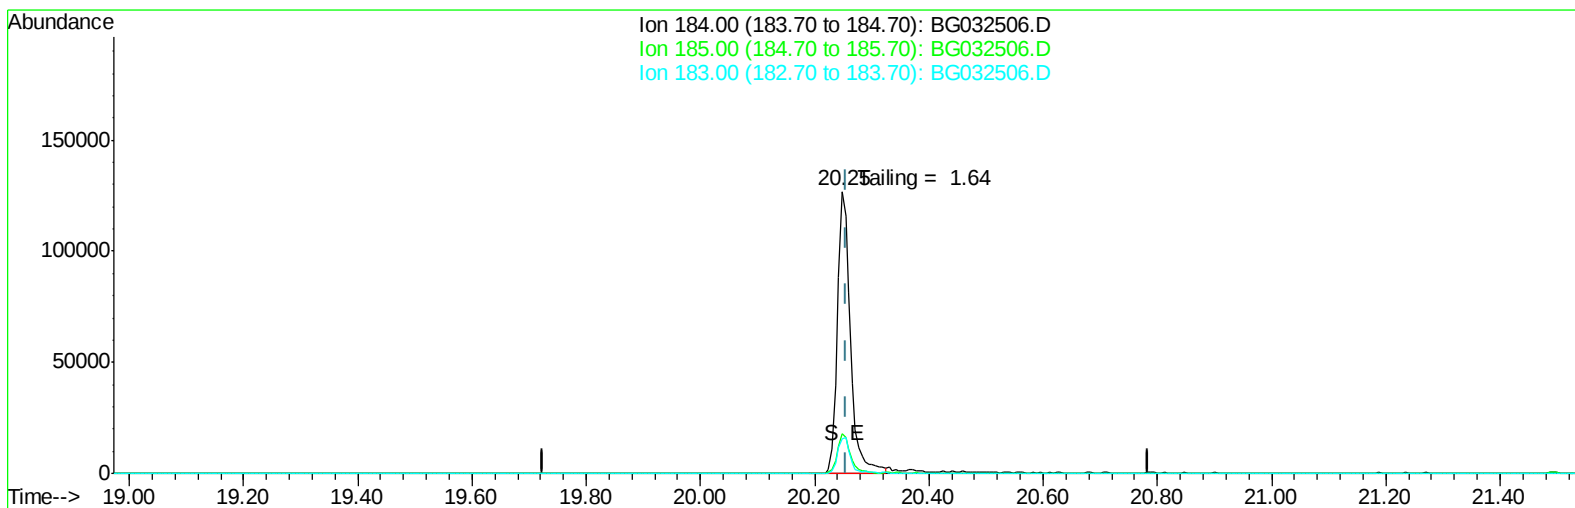

TIC: BG032506.D

(76) Benzidine

20.248min (-0.007) 0.00ng

response 203439

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.90
183.00	13.30	12.25
0.00	0.00	0.00