
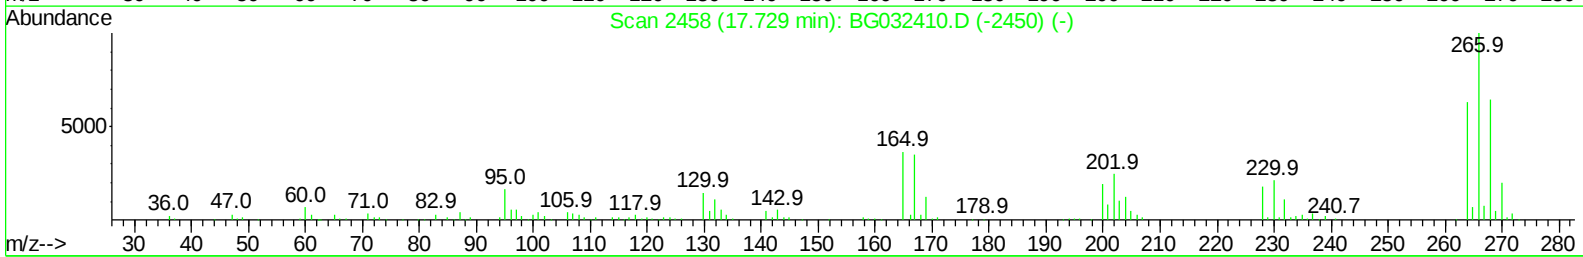
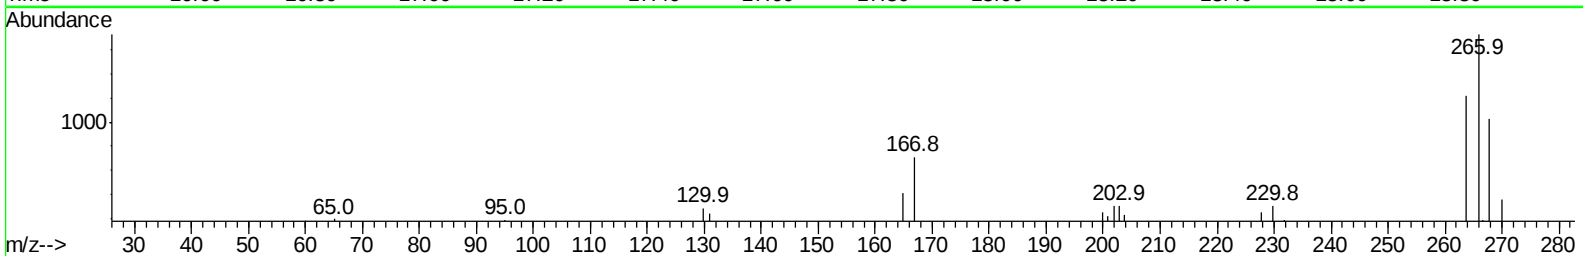


Data Path : U:\HPCHEM1\BNA G\DATA\BG020218\
Data File : BG032523.D
Acq On : 2 Feb 2018 22:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 00:12:11 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

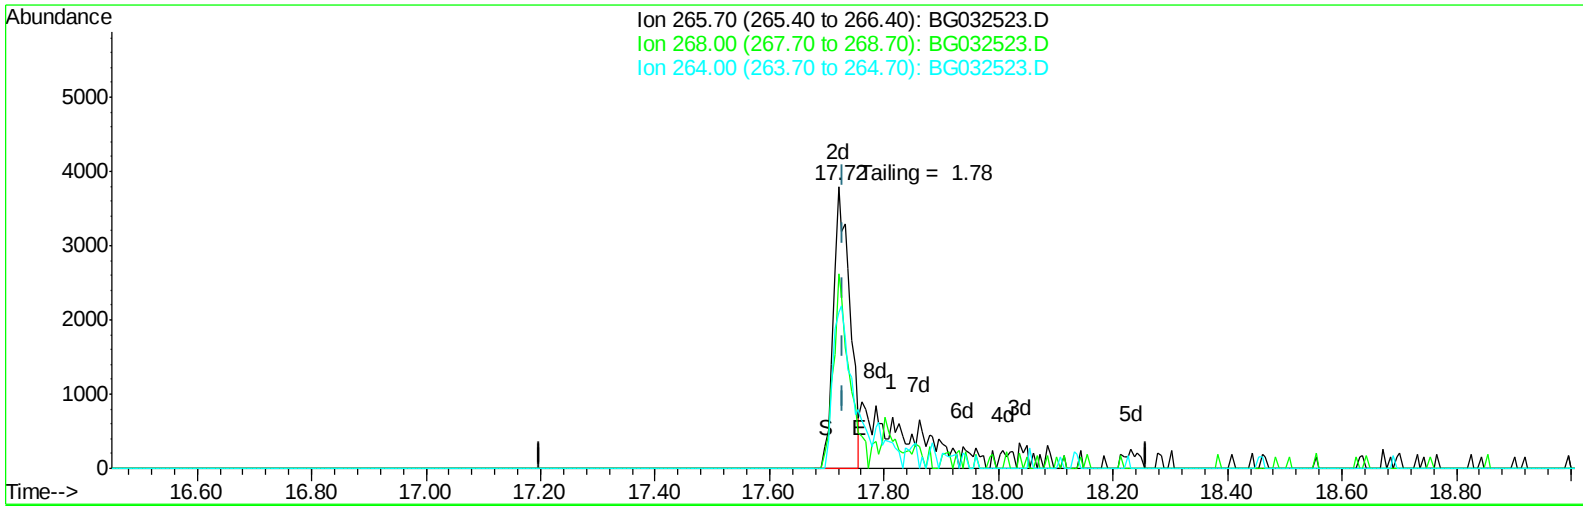

TIC: BG032523.D

(69) Pentachlorophenol (C)




17.814min (+0.086) 211.73ng

response 548

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	52.35
264.00	62.00	51.76
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG020218\
Data File : BG032512.D
Acq On : 2 Feb 2018 15:07
Operator : SJ/JU
Sample : J1429-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 02 22:23:43 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

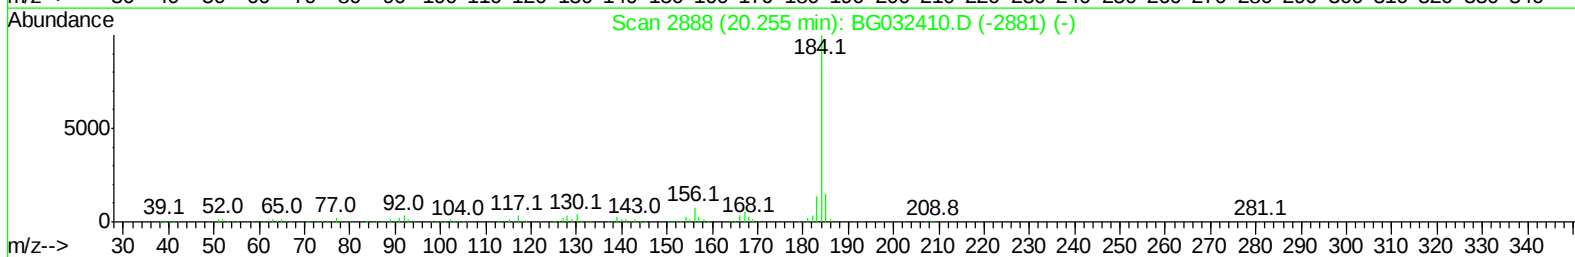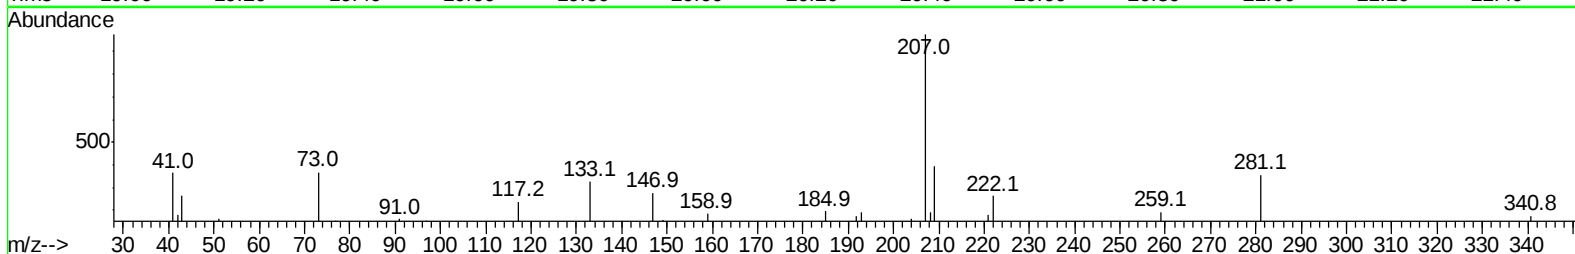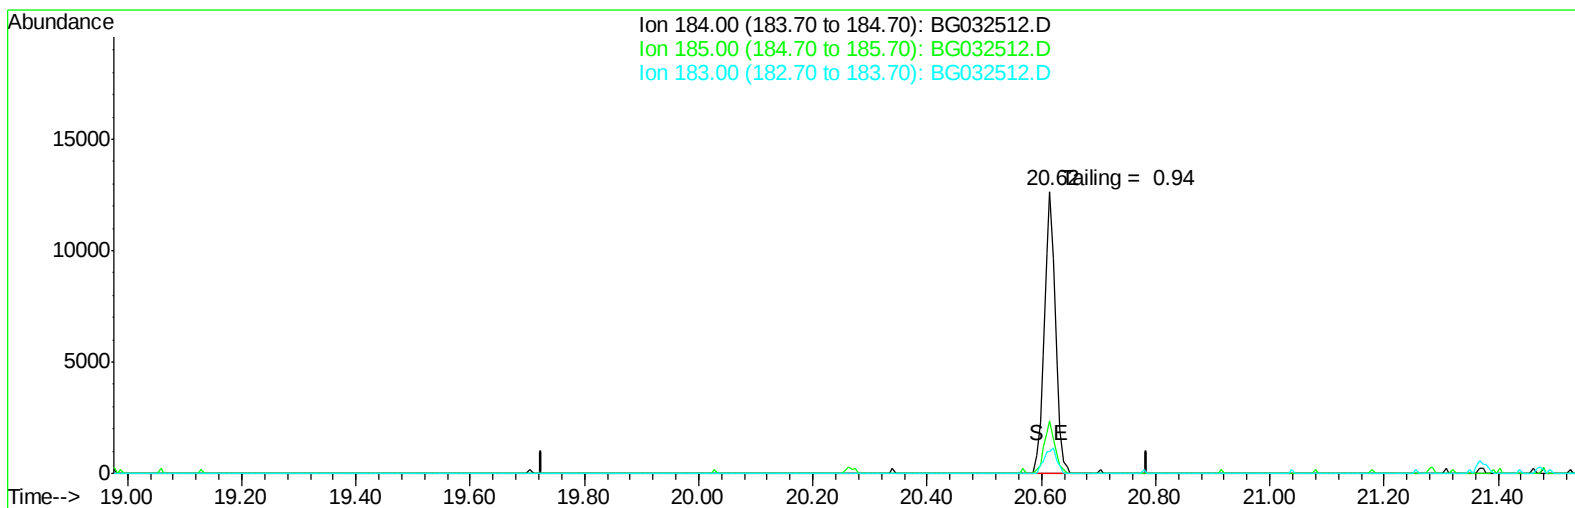

TIC: BG032512.D

(76) Benzidine

20.255min (-20.255) 0.00ng d

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	13.90	0.00
183.00	13.30	0.00
0.00	0.00	0.00