

Data Path : U:\HPCHEM1\BNA G\DATA\BG020218\
Data File : BG032520.D
Acq On : 2 Feb 2018 20:09
Operator : SJ/JU
Sample : PB106274BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106274BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.149	479	487	501	rBV2	280428	552984	20.77%	5.523%
2	7.829	766	773	788	rBV	266706	580958	21.82%	5.802%
3	8.223	832	840	857	rBV	314066	653083	24.53%	6.522%
4	8.710	915	923	937	rBV	67957	139535	5.24%	1.394%
5	9.039	971	979	990	rBV	275497	555364	20.86%	5.546%
6	9.909	1118	1127	1138	rBV	163597	364299	13.68%	3.638%
7	11.584	1405	1412	1424	rBV	88001	191139	7.18%	1.909%
8	13.969	1810	1818	1836	rBV	719938	1230904	46.23%	12.293%
9	15.344	2044	2052	2064	rBV2	176345	316153	11.87%	3.157%
10	16.819	2296	2303	2317	rBV	493116	886792	33.31%	8.856%
11	18.076	2511	2517	2530	rBV2	281132	466925	17.54%	4.663%
12	20.614	2943	2949	2961	rBV	1994469	2662529	100.00%	26.590%
13	22.406	3246	3254	3263	rBV2	367339	702838	26.40%	7.019%
14	26.078	3866	3879	3898	rBV	209055	709712	26.66%	7.088%


Sum of corrected areas: 10013215

Data Path : U:\HPCHEM1\BNA G\DATA\BG020218\
Data File : BG032520.D
Acq On : 2 Feb 2018 20:09
Operator : SJ/JU
Sample : PB106274BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106274BL

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

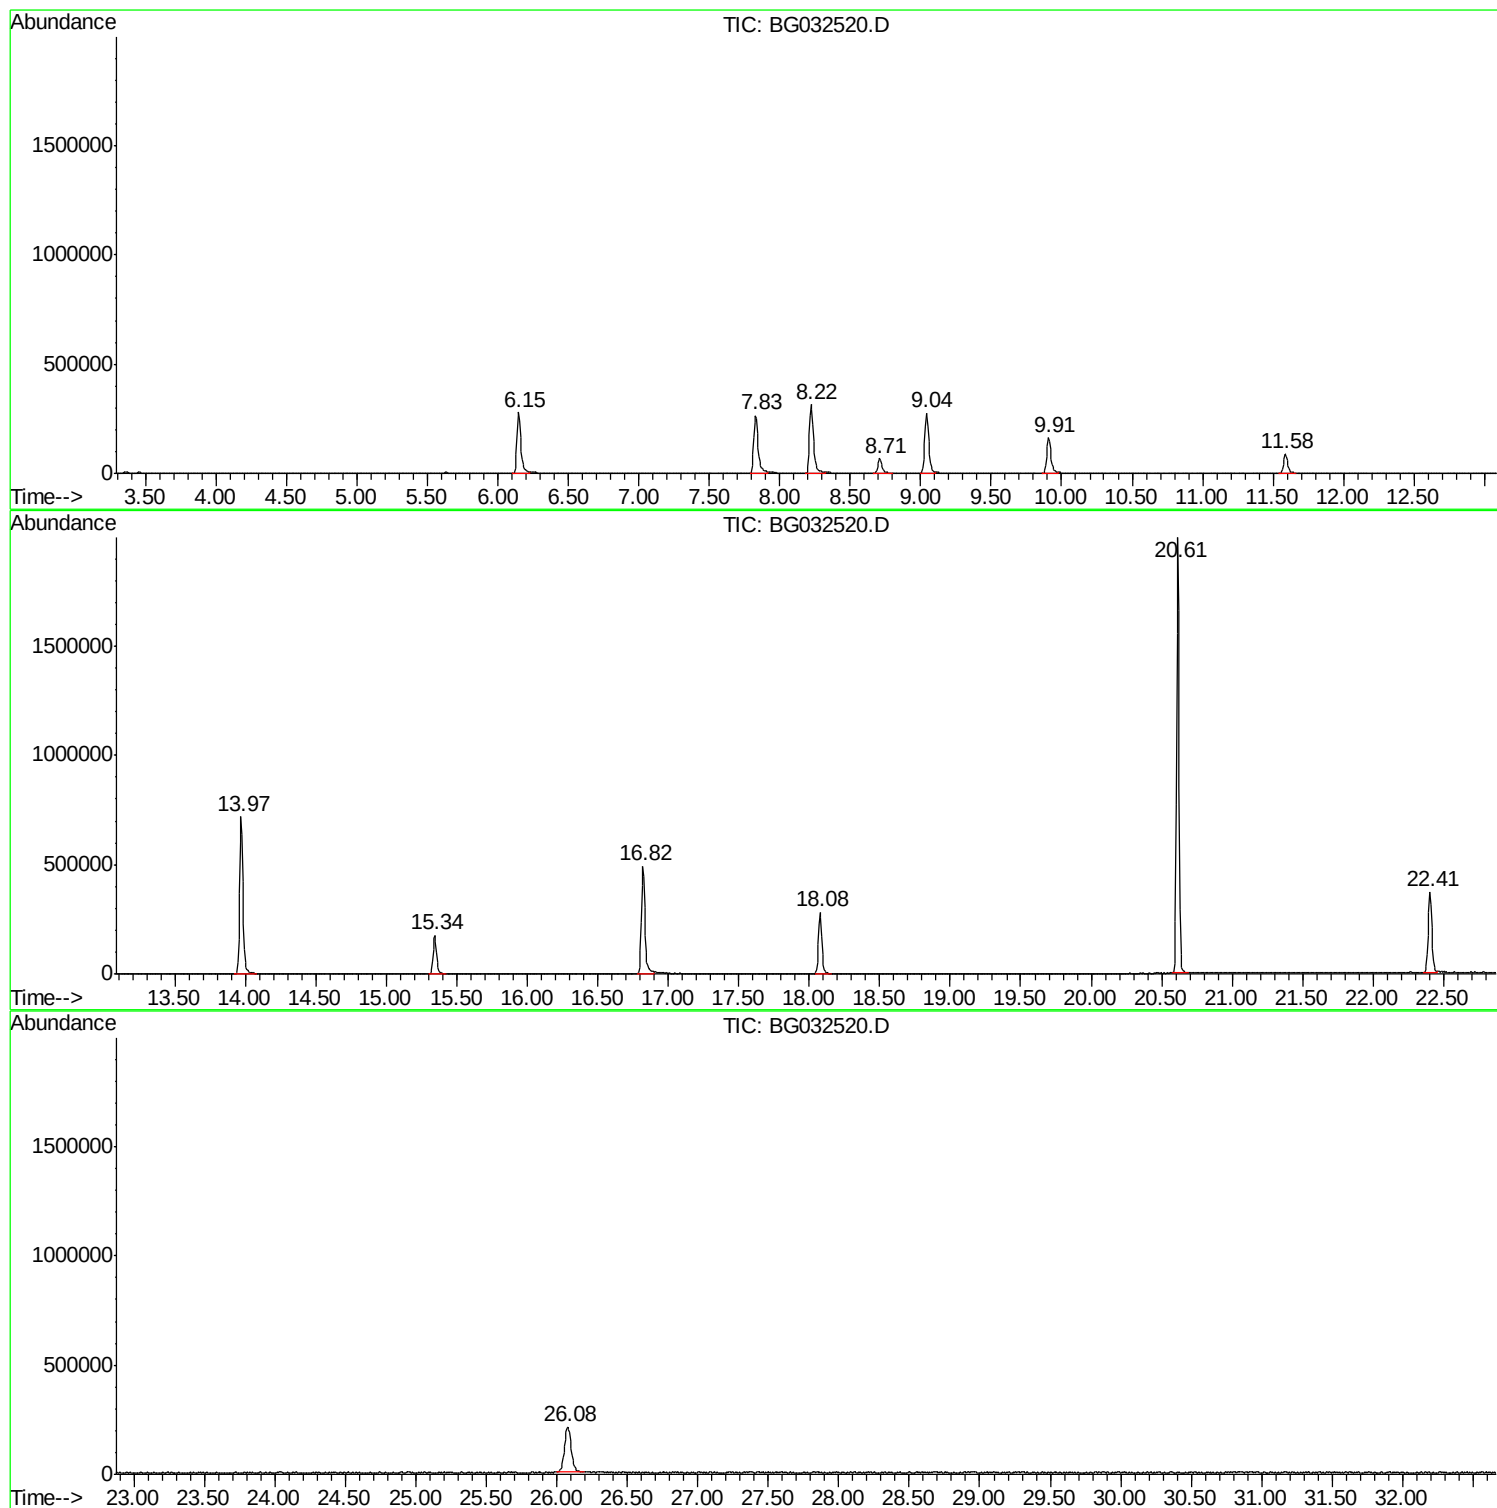

Data Path : U:\HPCHEM1\BNA G\DATA\BG020218\
Data File : BG032520.D
Acq On : 2 Feb 2018 20:09
Operator : SJ/JU
Sample : PB106274BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106274BL










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown8.22 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.22	93.61 ng	653083	1,4-Dichlorobenzene-d4	8.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	35
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	12

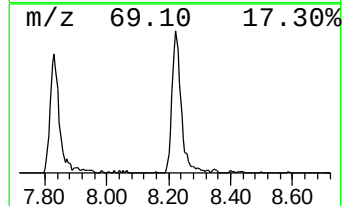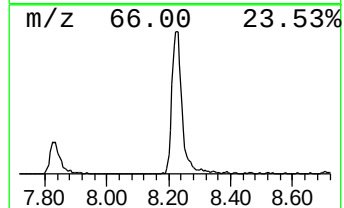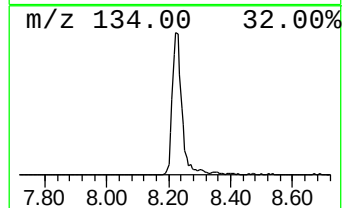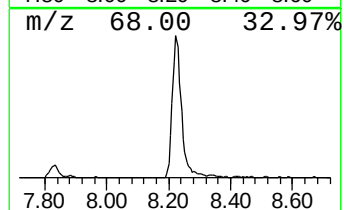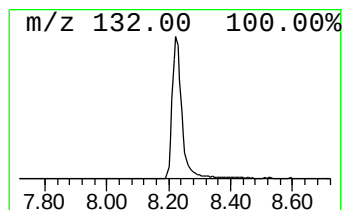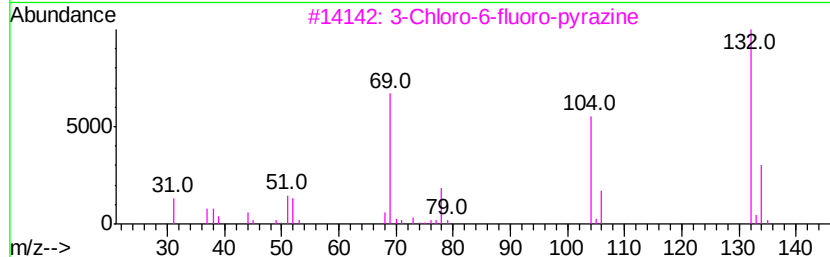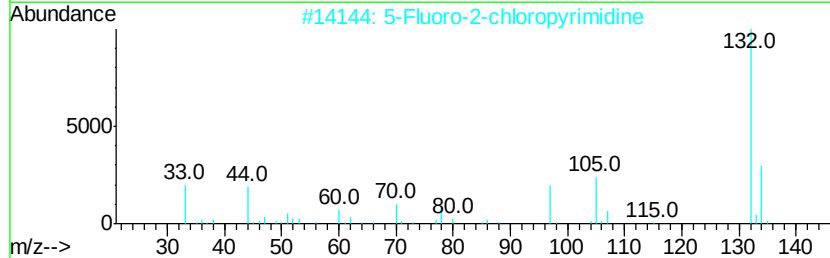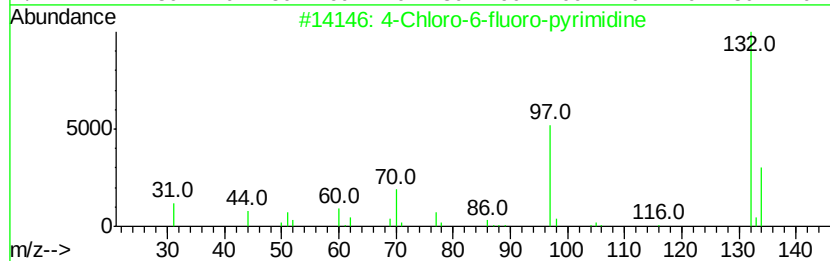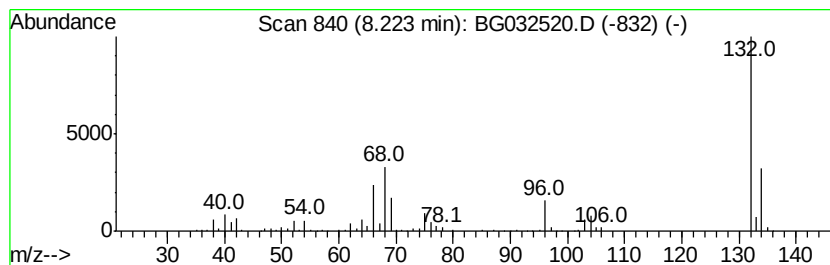

Data Path : U:\HPCHEM1\BNA_G\DATA\BG020218\
Data File : BG032520.D
Acq On : 2 Feb 2018 20:09
Operator : SJ/JU
Sample : PB106274BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106274BL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.22	8.22	93.6	ng	653083	1	8.71	139535	20.0