

Data Path : U:\HPCHEM1\BNA G\DATA\BG020218\
 Data File : BG032522.D
 Acq On : 2 Feb 2018 21:24
 Operator : SJ/JU
 Sample : PB106268BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB106268BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.146	479	486	505	rBV	259396	522640	19.69%	5.487%
2	7.827	765	772	793	rBV	245608	553010	20.83%	5.806%
3	8.226	832	840	856	rBV	284407	607703	22.89%	6.380%
4	8.708	915	922	935	rBV2	57820	123989	4.67%	1.302%
5	9.043	971	979	996	rBV	271061	522529	19.69%	5.486%
6	9.907	1118	1126	1141	rBV2	155213	338961	12.77%	3.559%
7	11.587	1404	1412	1423	rBV	75038	168033	6.33%	1.764%
8	13.972	1810	1818	1835	rBV	655250	1158850	43.66%	12.167%
9	15.341	2043	2051	2070	rVB	158543	289163	10.89%	3.036%
10	16.822	2296	2303	2317	rBV	450873	838882	31.60%	8.807%
11	18.079	2509	2517	2527	rBV	242542	424159	15.98%	4.453%
12	20.618	2942	2949	2963	rBV	1922685	2654430	100.00%	27.868%
13	22.404	3244	3253	3264	rBV2	333006	656426	24.73%	6.892%
14	26.082	3867	3879	3898	rBV2	192070	666123	25.09%	6.993%


Sum of corrected areas: 9524898

Data Path : U:\HPCHEM1\BNA G\DATA\BG020218\
Data File : BG032522.D
Acq On : 2 Feb 2018 21:24
Operator : SJ/JU
Sample : PB106268BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106268BL

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

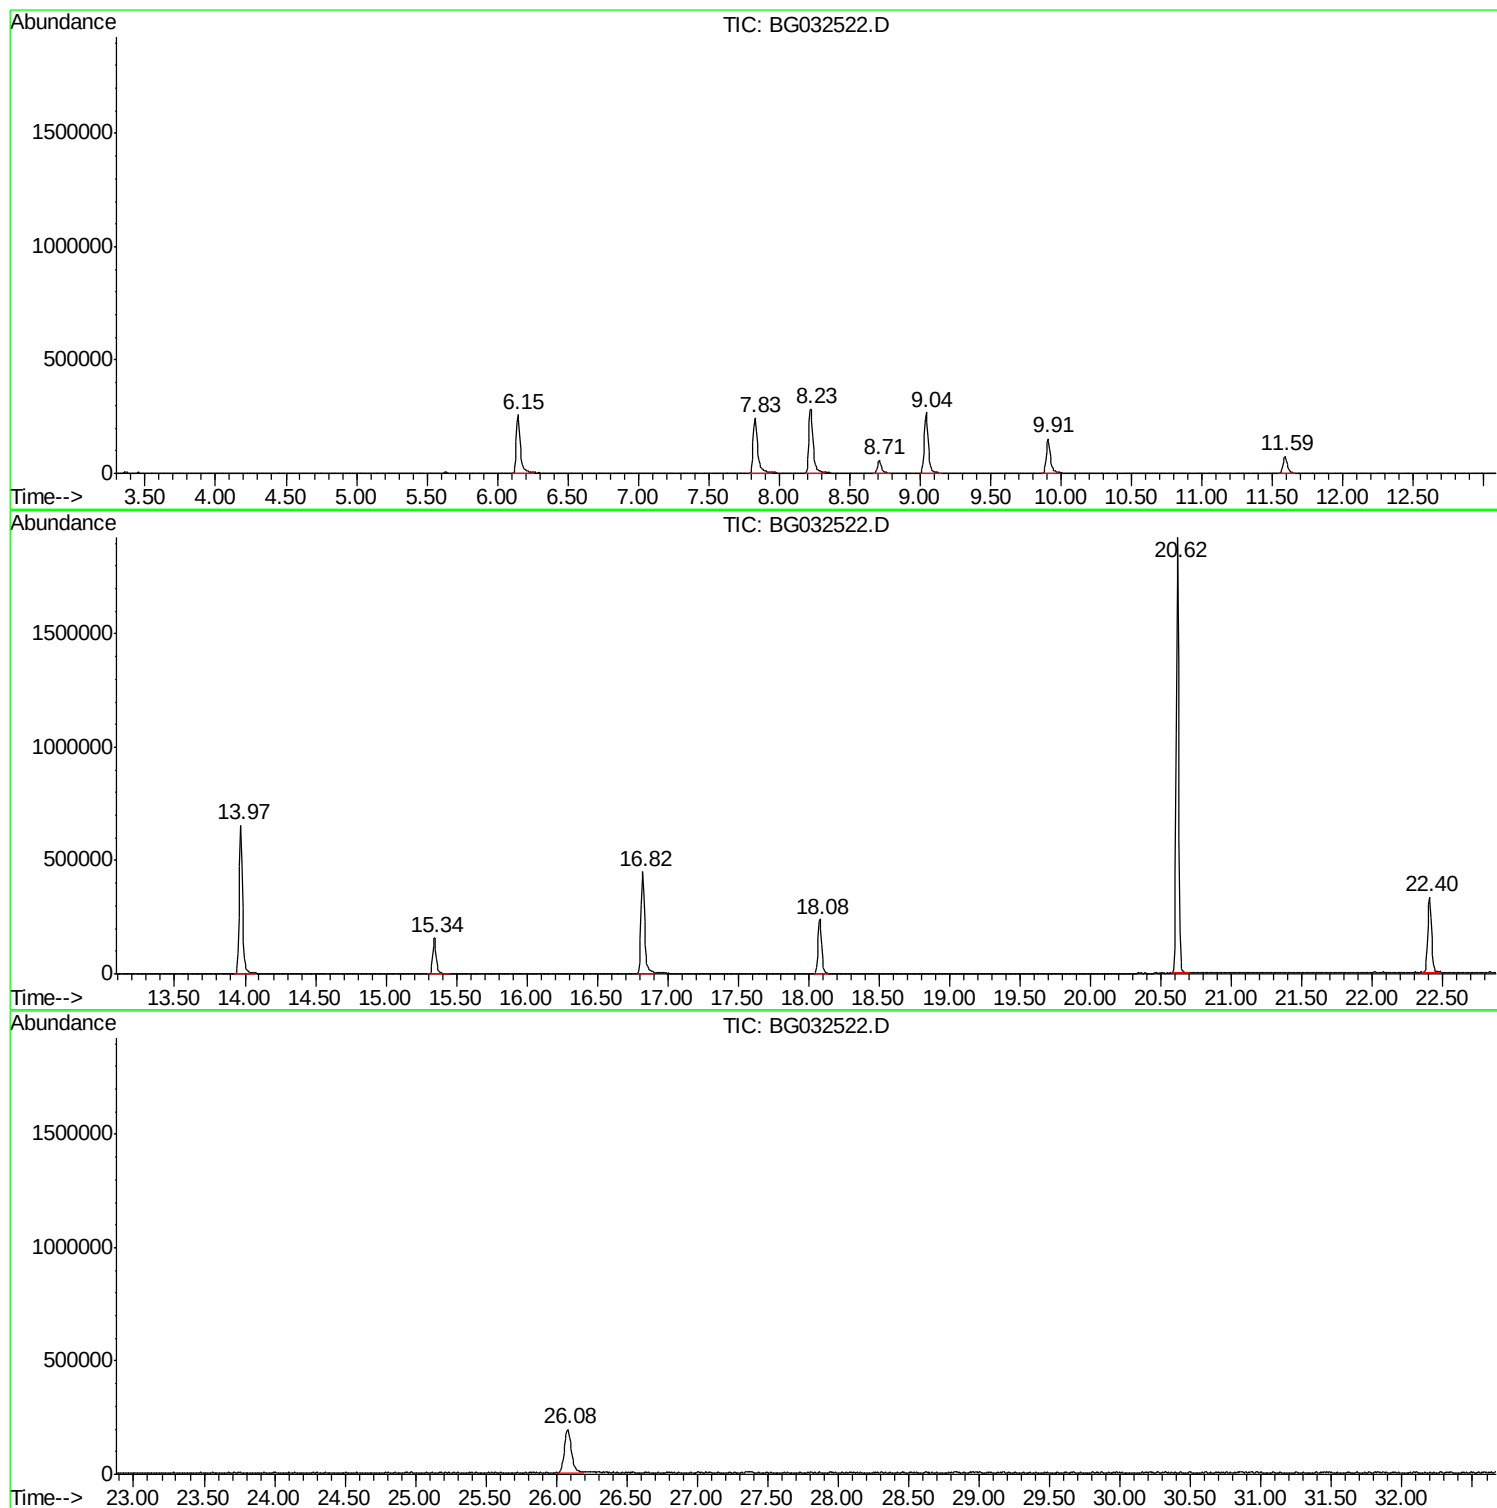

Data Path : U:\HPCHEM1\BNA G\DATA\BG020218\
Data File : BG032522.D
Acq On : 2 Feb 2018 21:24
Operator : SJ/JU
Sample : PB106268BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106268BL










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown8.23 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.23	98.03 ng	607703	1,4-Dichlorobenzene-d4	8.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	35
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	17
4		5-Aminoindole	132	C8H8N2	005192-03-0	16
5		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	10

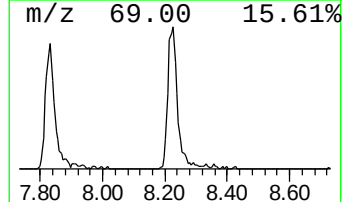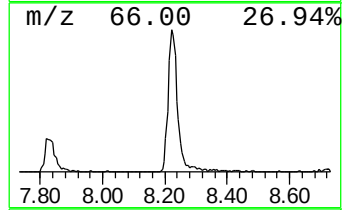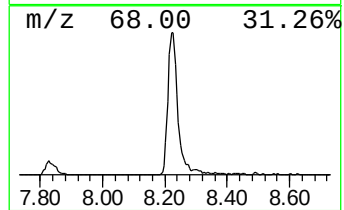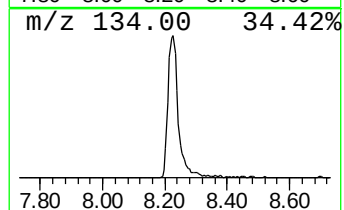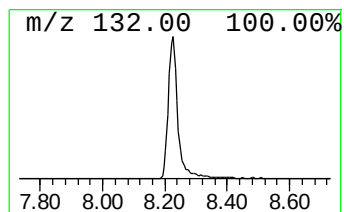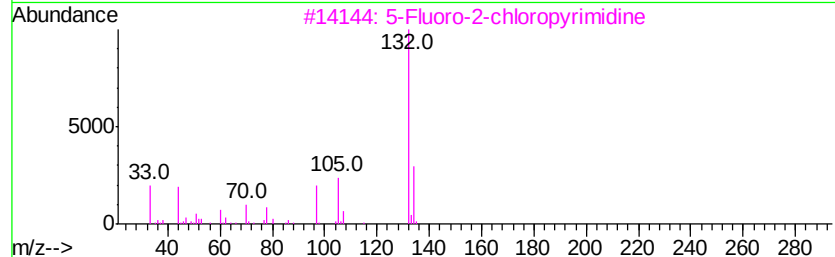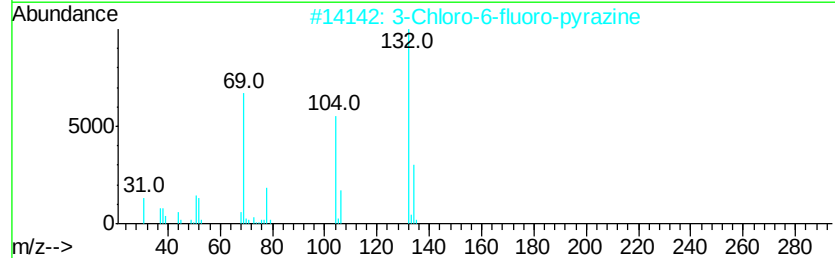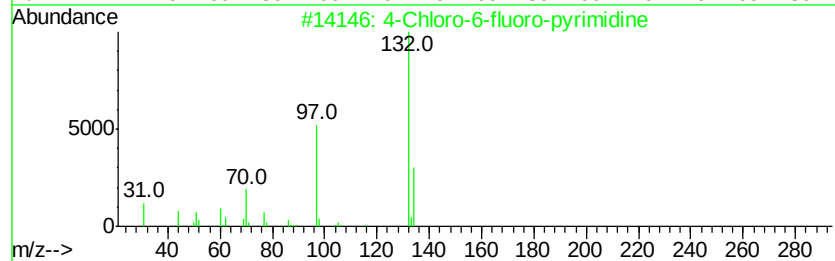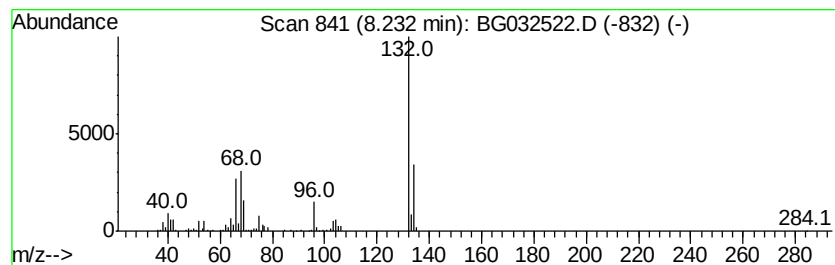

Data Path : U:\HPCHEM1\BNA_G\DATA\BG020218\
Data File : BG032522.D
Acq On : 2 Feb 2018 21:24
Operator : SJ/JU
Sample : PB106268BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106268BL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.23	8.23	98.0	ng	607703	1	8.71	123989	20.0