


Data Path : U:\HPCHEM1\BNA G\Data\BG020218\
 Data File : BG032506.D
 Acq On : 2 Feb 2018 10:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 29 15:32:55 2018

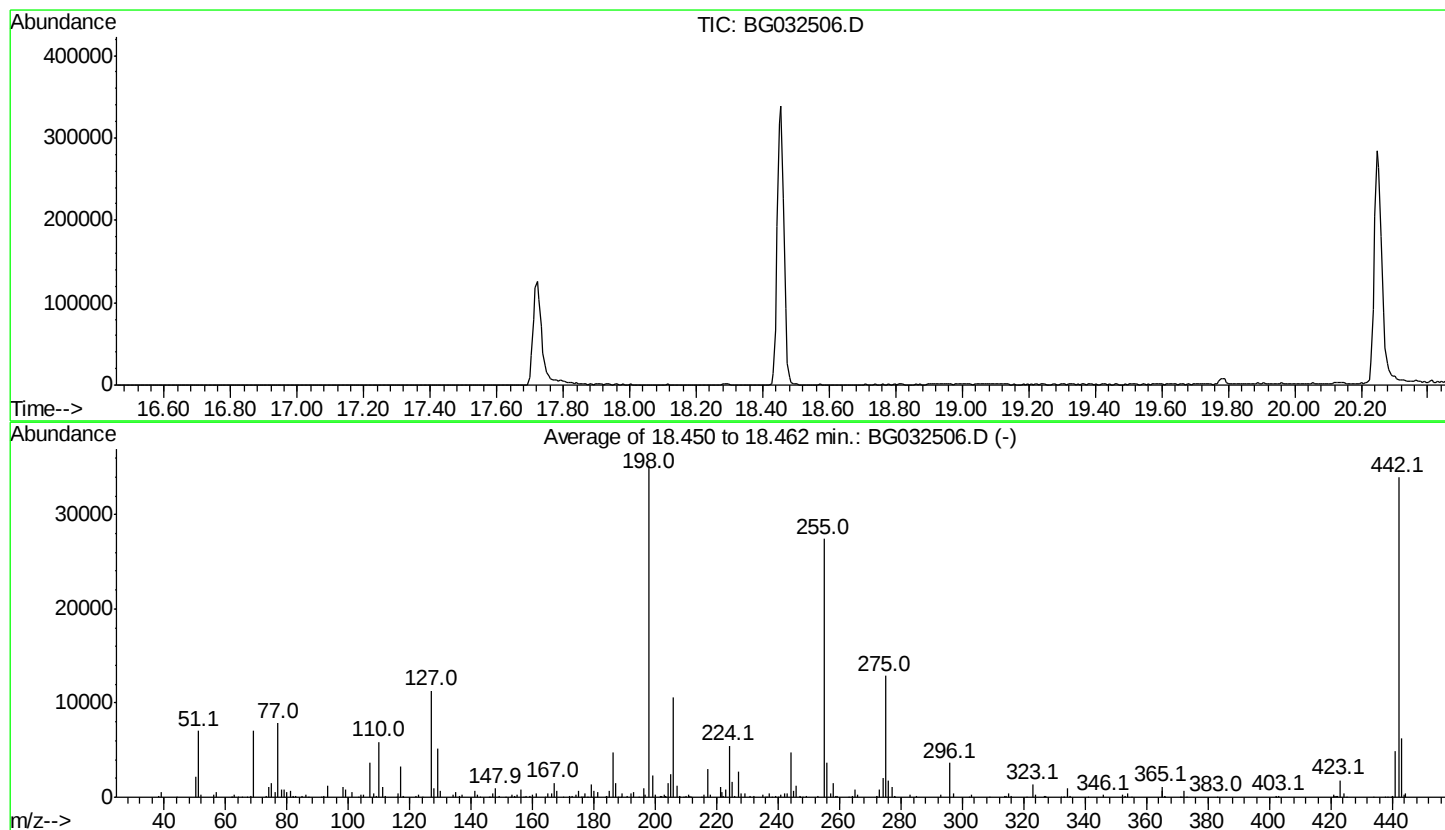

AutoFind: Scans 2580, 2581, 2582; Background Corrected with Scan 2573

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.9	7006	PASS
68	69	0.00	2	1.5	105	PASS
69	198	0.00	100	20.0	7055	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.2	11322	PASS
197	198	0.00	2	0.8	293	PASS
198	198	100	100	100.0	35197	PASS
199	198	5	9	6.6	2314	PASS
275	198	10	60	36.6	12885	PASS
365	198	1	100	3.2	1113	PASS
441	442	0.01	24	14.4	4900	PASS
442	198	50	100	96.5	33954	PASS
443	442	15	24	18.5	6290	PASS