


Data Path : U:\HPCHEM1\BNA G\Data\BG020218\
 Data File : BG032523.D
 Acq On : 2 Feb 2018 22:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 29 15:32:55 2018

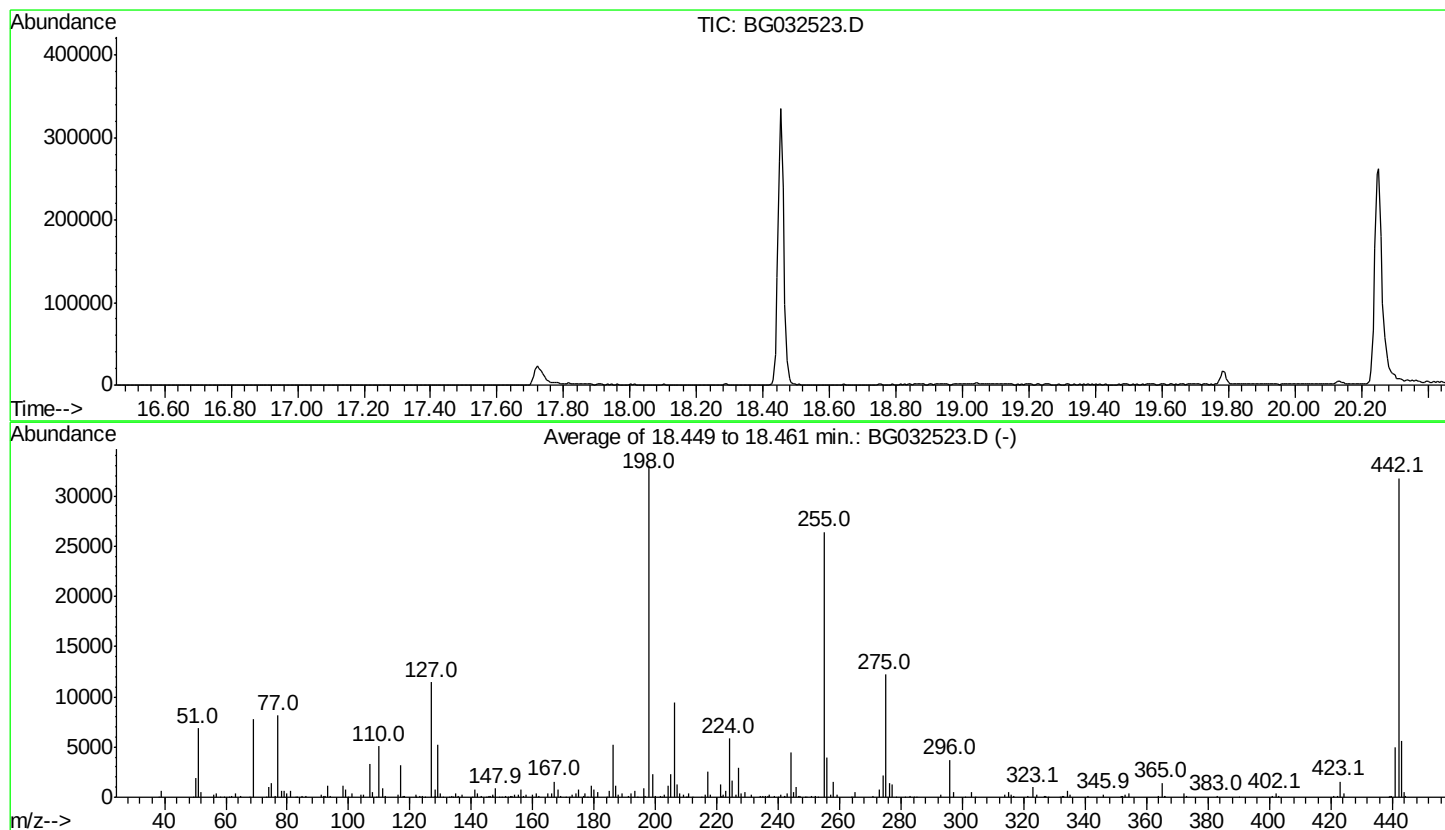

AutoFind: Scans 2580, 2581, 2582; Background Corrected with Scan 2573

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.8	6859	PASS
68	69	0.00	2	0.7	52	PASS
69	198	0.00	100	23.5	7743	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	34.7	11462	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33005	PASS
199	198	5	9	7.0	2299	PASS
275	198	10	60	37.0	12216	PASS
365	198	1	100	4.4	1446	PASS
441	442	0.01	24	15.5	4918	PASS
442	198	50	100	96.3	31768	PASS
443	442	15	24	17.8	5667	PASS