
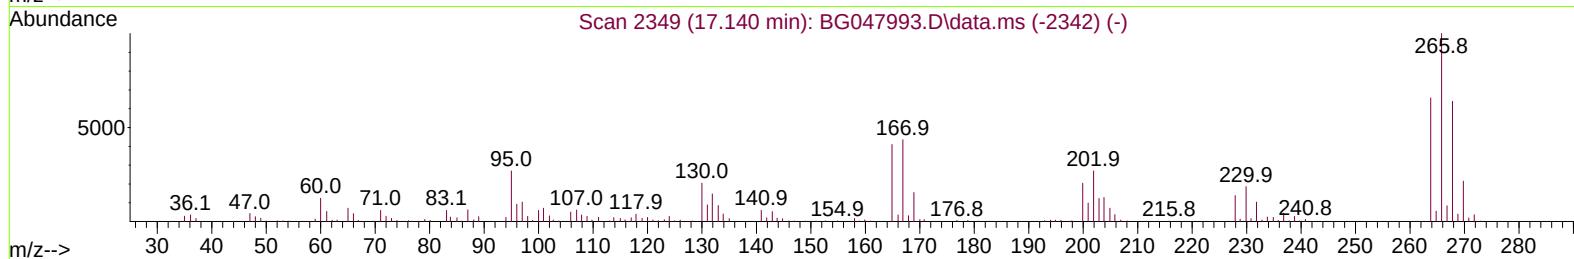
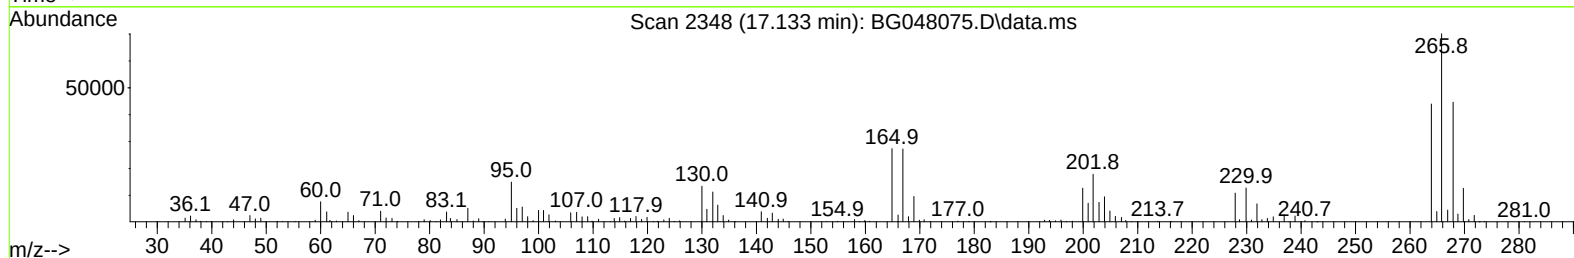


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020221\
Data File : BG048075.D
Acq On : 2 Feb 2021 12:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 01:13:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 02 15:30:13 2021
Response via : Initial Calibration

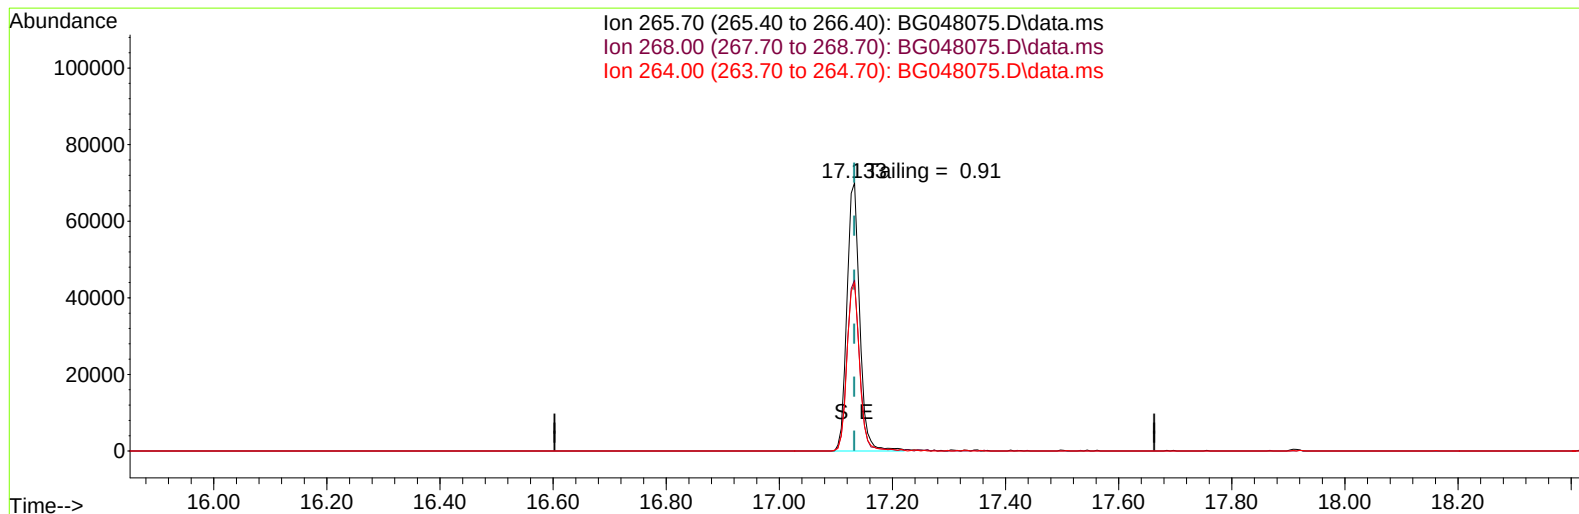

TIC: BG048075.D\data.ms

(70) Pentachlorophenol (C)




17.133min (+ 0.000) 227593.89 ng

response 110453

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.67
264.00	61.60	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020221\
 Data File : BG048075.D
 Acq On : 2 Feb 2021 12:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 01:13:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 02 15:30:13 2021
 Response via : Initial Calibration

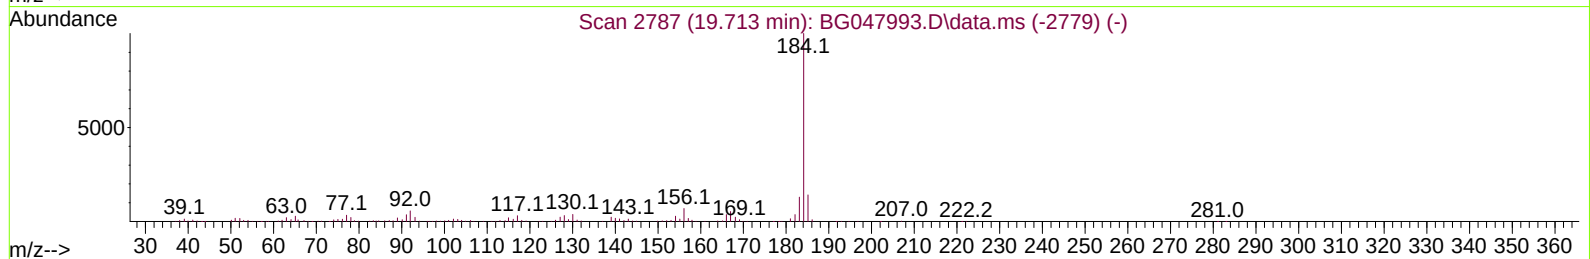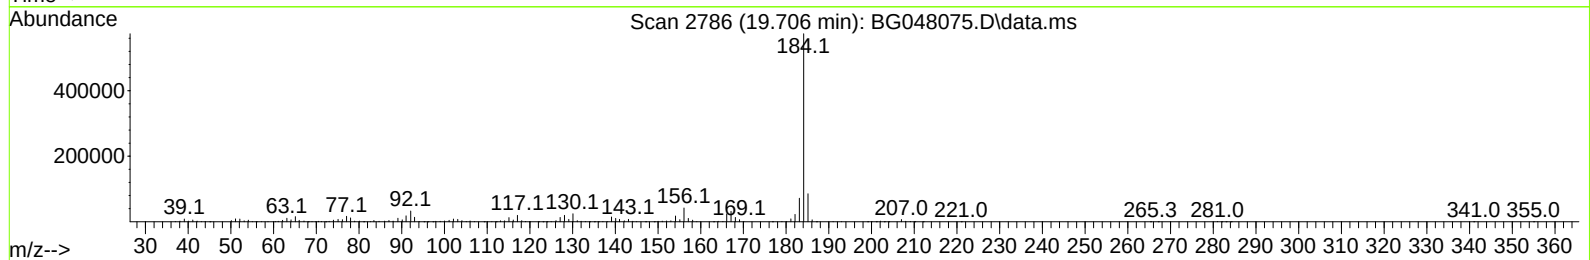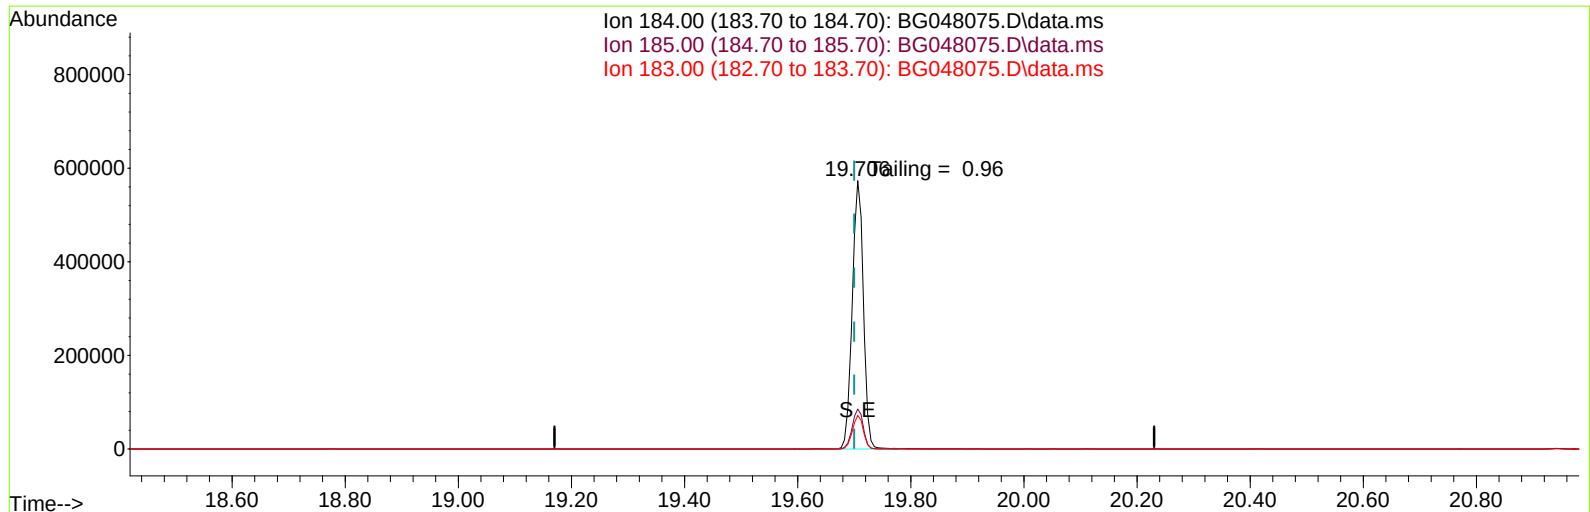

TIC: BG048075.D\data.ms

(77) Benzidine**19.706min (+ 0.006) 3529.13 ng****response 787284**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.93
183.00	13.20	12.51
0.00	0.00	0.00