
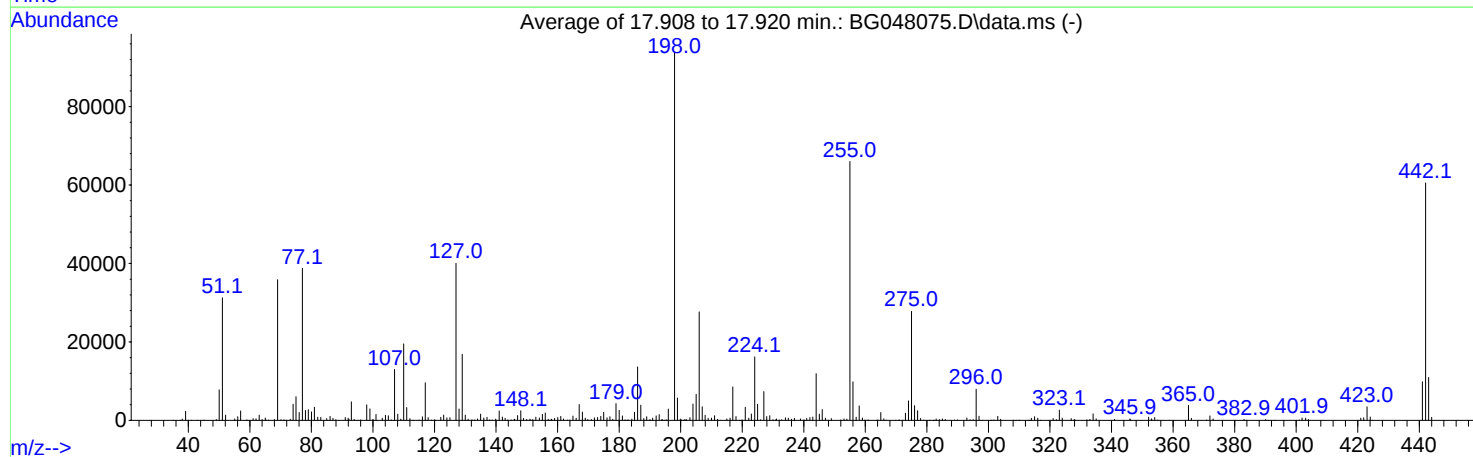


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020221\  
 Data File : BG048075.D  
 Acq On : 2 Feb 2021 12:47  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG012521.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Feb 02 15:30:13 2021

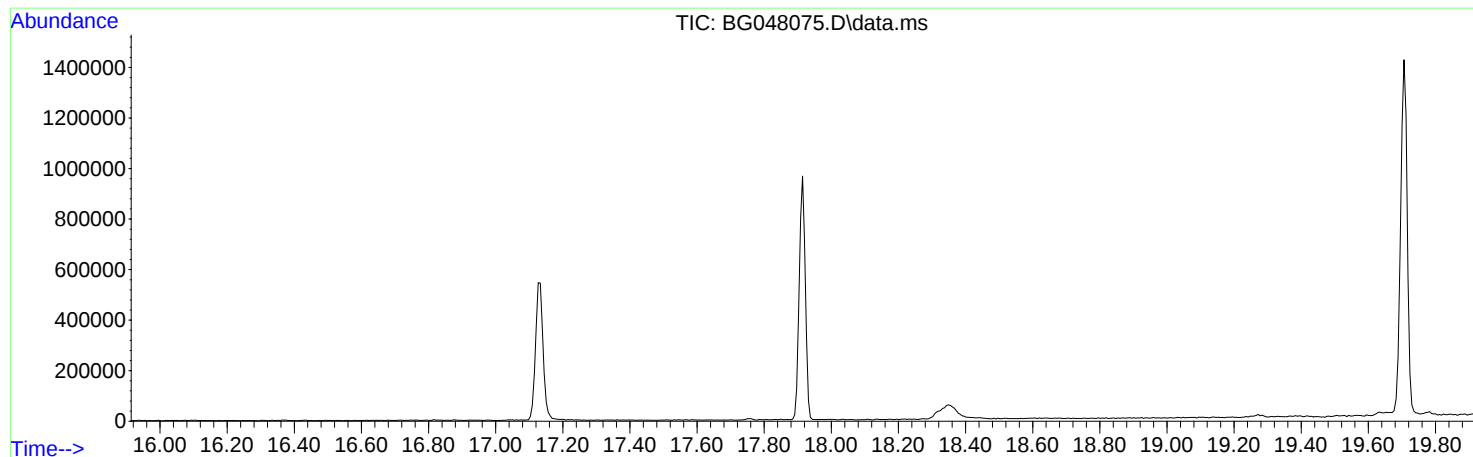




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 33.3         | 31245      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.6          | 215        | PASS                |
| 69             | 198             | 0.00            | 100             | 38.3         | 35877      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 182        | PASS                |
| 127            | 198             | 10              | 80              | 42.7         | 40048      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 93784      | PASS                |
| 199            | 198             | 5               | 9               | 6.1          | 5704       | PASS                |
| 275            | 198             | 10              | 60              | 29.6         | 27797      | PASS                |
| 365            | 198             | 1               | 100             | 4.1          | 3799       | PASS                |
| 441            | 198             | 0.01            | 100             | 10.5         | 9854       | PASS                |
| 442            | 198             | 50              | 100             | 64.5         | 60531      | PASS                |
| 443            | 442             | 15              | 24              | 18.1         | 10932      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020221\  
Data File : BG048075.D  
Acq On : 2 Feb 2021 12:47  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Feb 03 01:13:22 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG012521.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 02 15:30:13 2021  
Response via : Initial Calibration

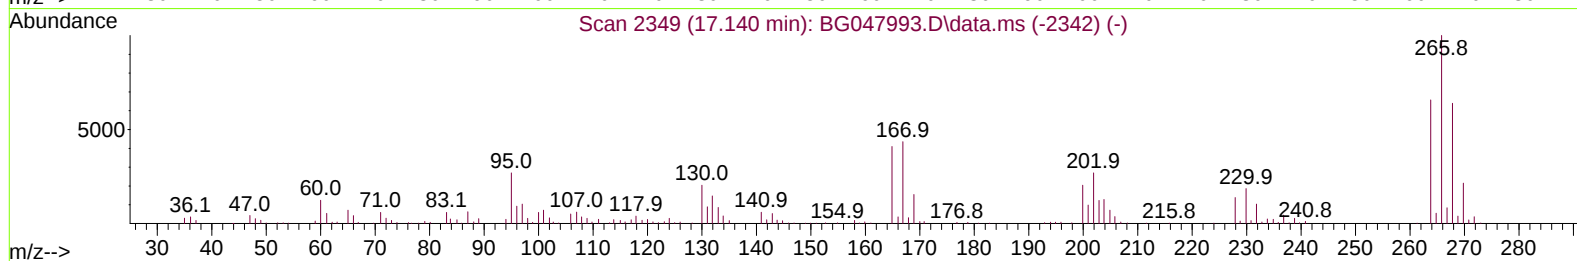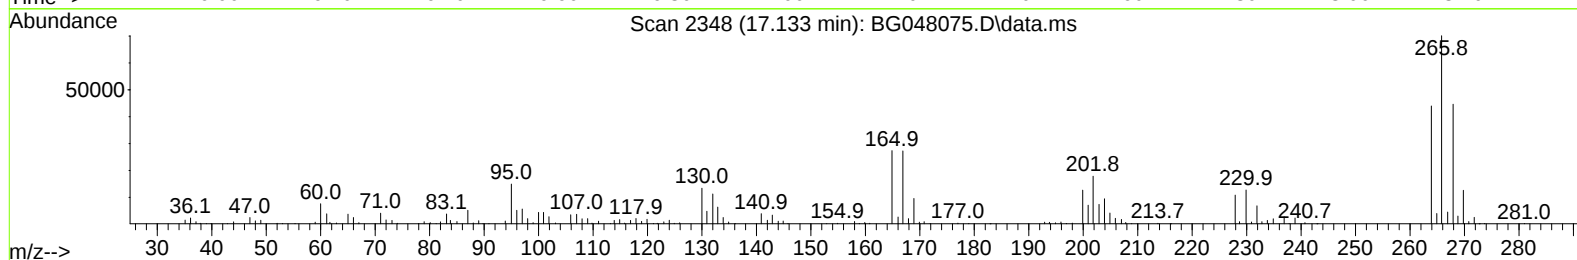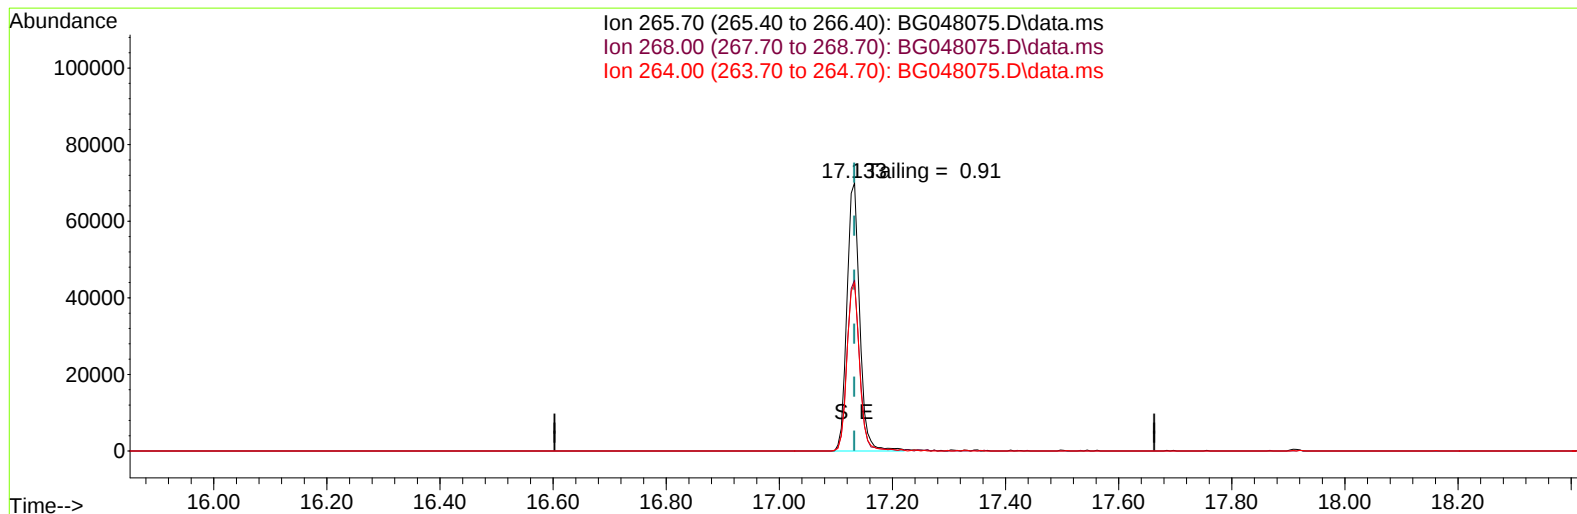

TIC: BG048075.D\data.ms

**(70) Pentachlorophenol (C)**

**17.133min (+ 0.000) 227593.89 ng**




**response 110453**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.67  |
| 264.00 | 61.60  | 62.71  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020221\  
Data File : BG048075.D  
Acq On : 2 Feb 2021 12:47  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Feb 03 01:13:22 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG012521.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 02 15:30:13 2021  
Response via : Initial Calibration

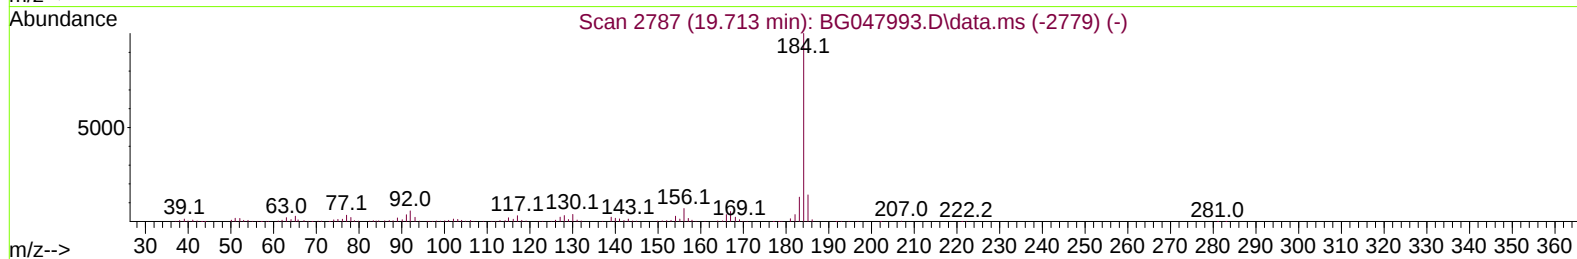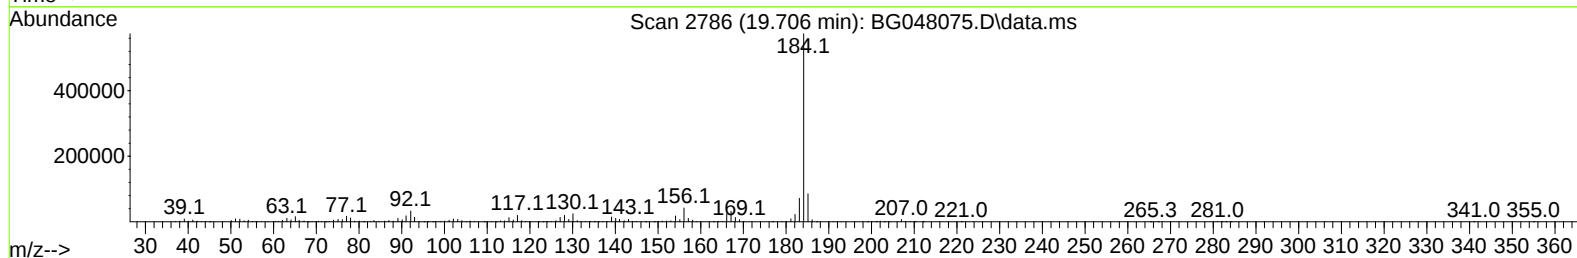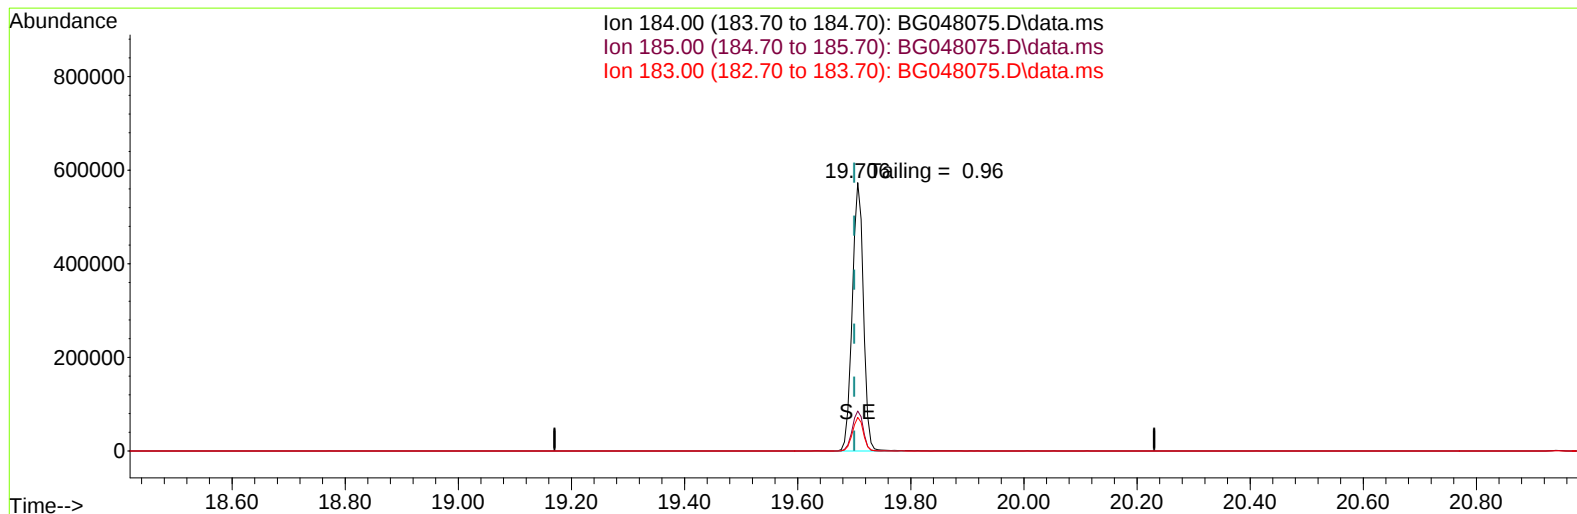

TIC: BG048075.D\data.ms

**(77) Benzidine**

**19.706min (+ 0.006) 3529.13 ng**

**response 787284**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.93  |
| 183.00 | 13.20  | 12.51  |
| 0.00   | 0.00   | 0.00   |

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 2/2/2021      | BNA_G            | <u>BG048075.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 381782           | 20.94              |
| DDD           | 3011             | 20.552             |
| DDE           | 427              | 19.994             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3438          | 385220           | 0.89               |
|               |                  |                    |