
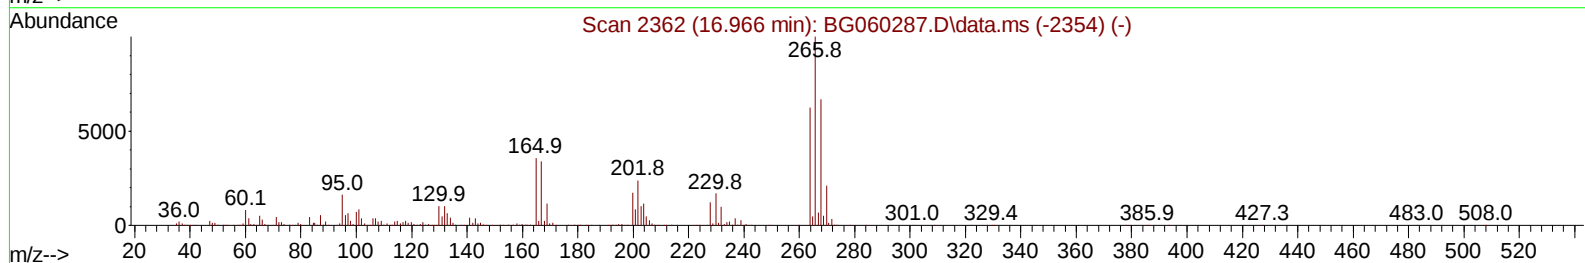
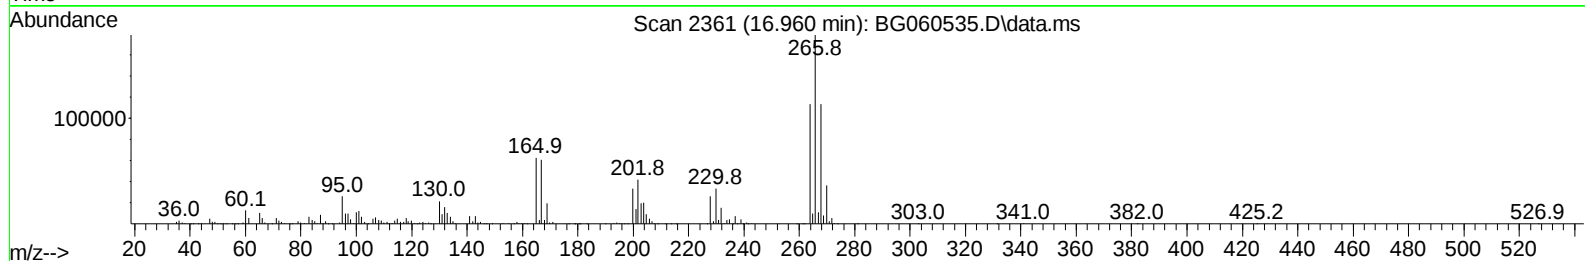


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020224\
Data File : BG060535.D
Acq On : 1 Feb 2024 15:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 01:08:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

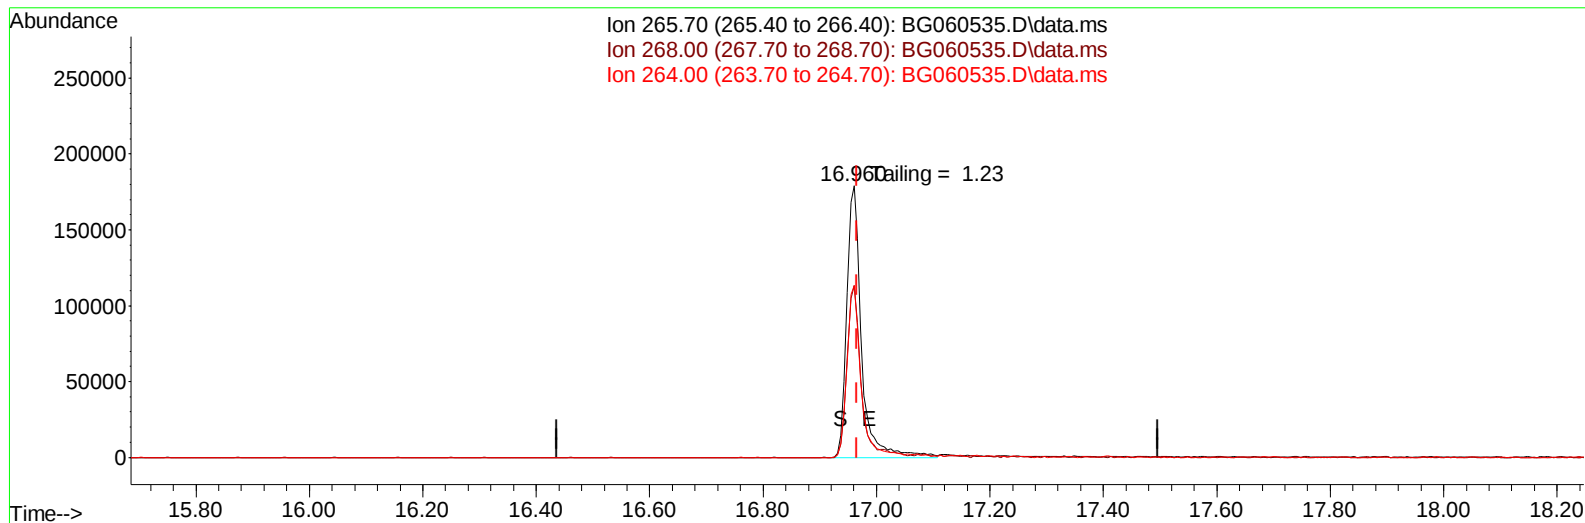

TIC: BG060535.D\data.ms

(70) Pentachlorophenol (C)




16.960min (-0.006) 798052.99 ng

response 324511

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	63.30
264.00	62.30	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020224\
Data File : BG060535.D
Acq On : 1 Feb 2024 15:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 01:08:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

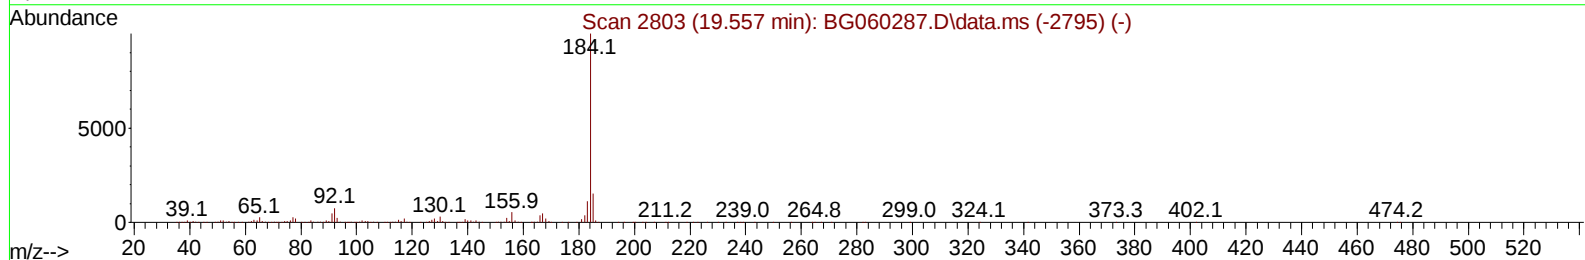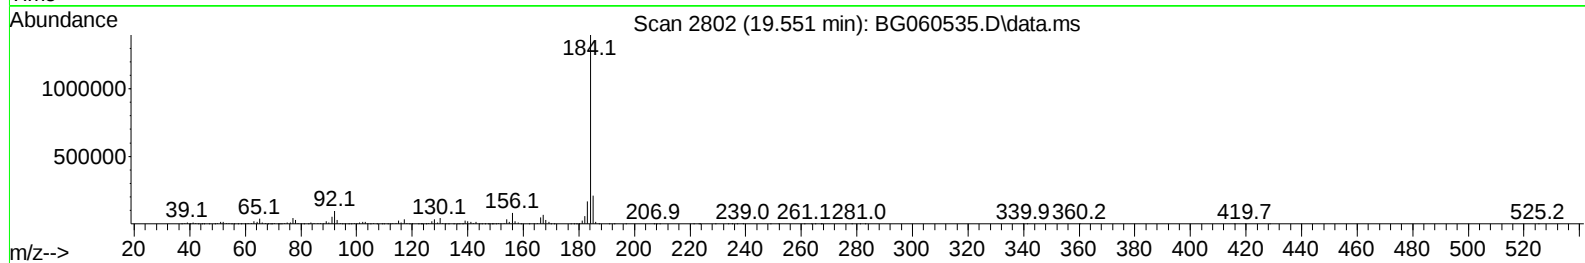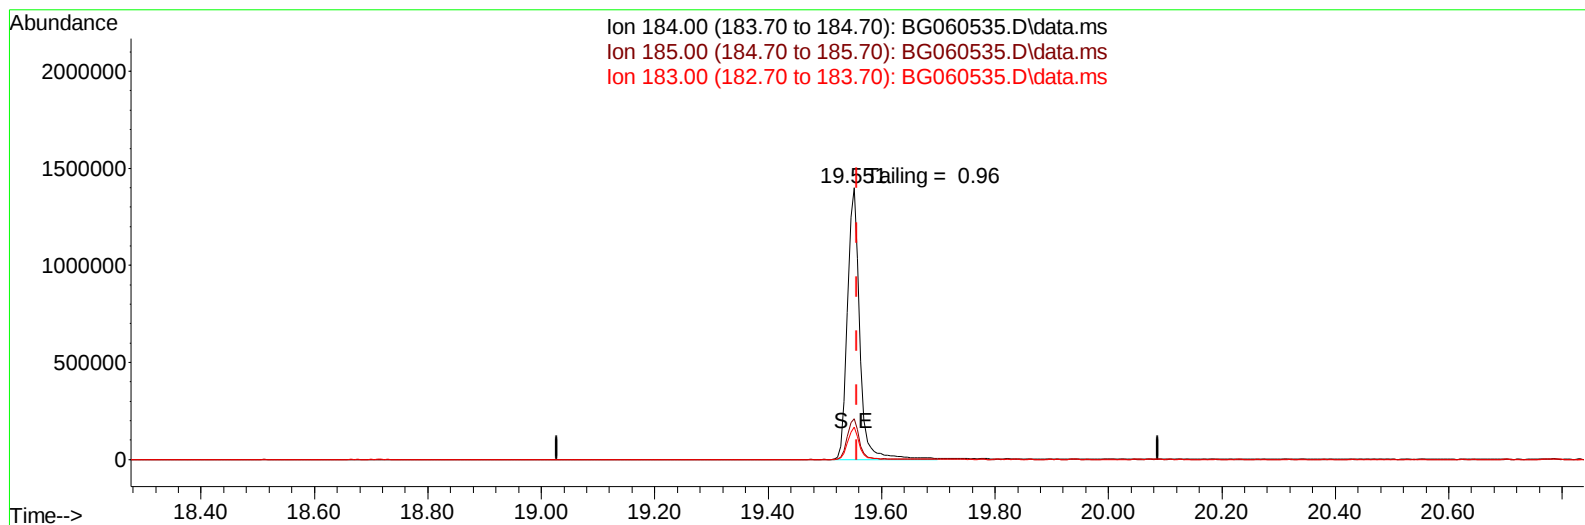

TIC: BG060535.D\data.ms

(77) Benzidine**19.551min (-0.006) 468842.84 ng****response 2118627**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	15.03
183.00	11.20	11.83
0.00	0.00	0.00