
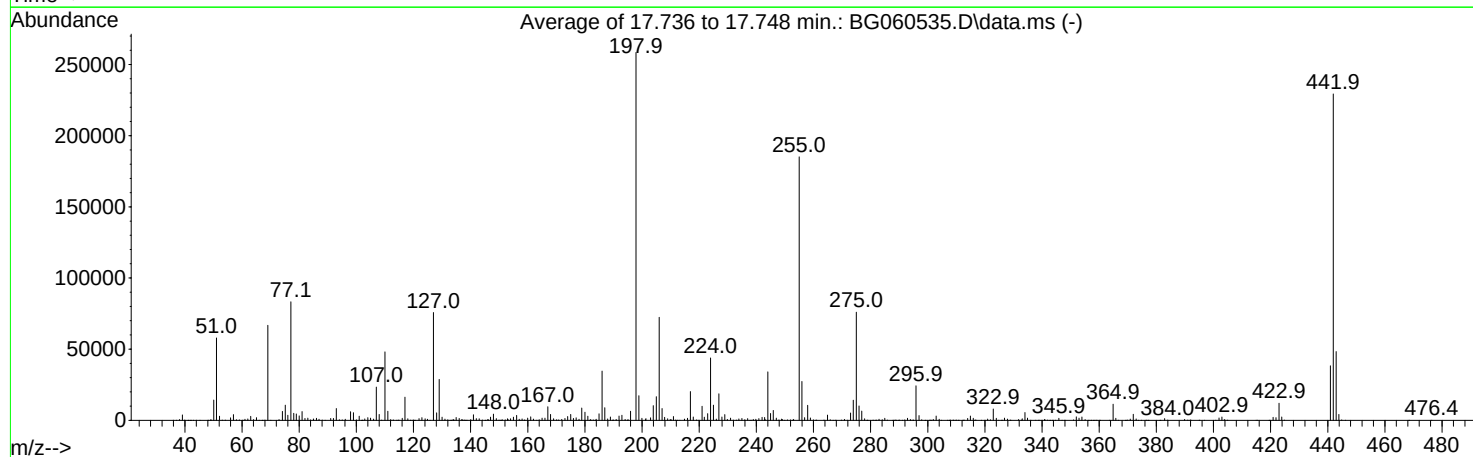


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020224\
Data File : BG060535.D
Acq On : 1 Feb 2024 15:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

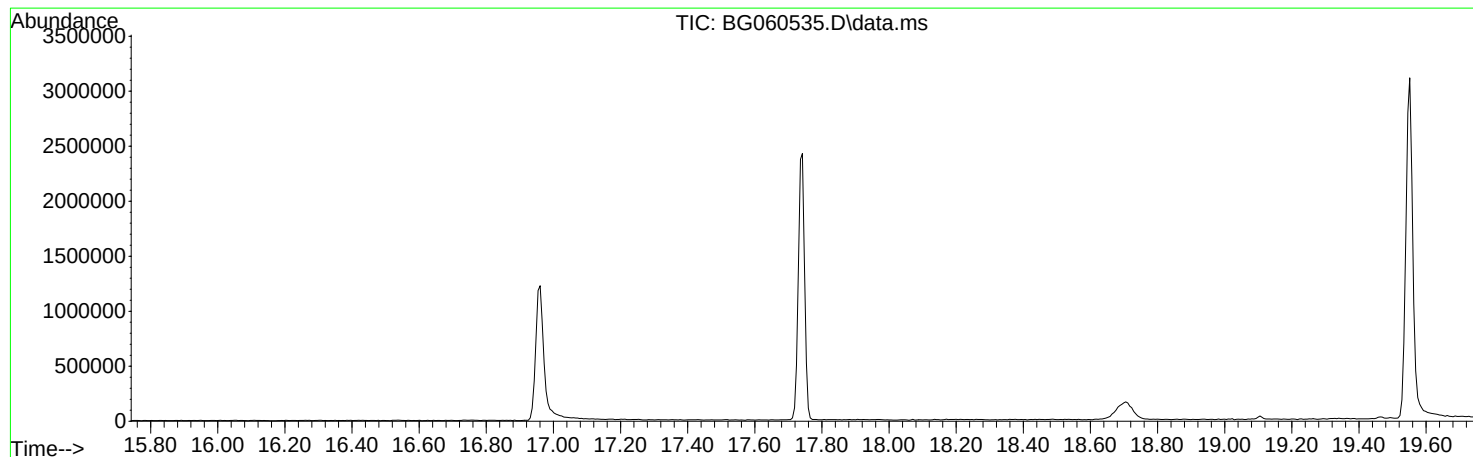




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	57891	PASS
68	69	0.00	2	0.4	281	PASS
69	198	0.00	100	25.8	66738	PASS
70	69	0.00	2	0.1	93	PASS
127	198	10	80	29.3	75744	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	258432	PASS
199	198	5	9	6.7	17329	PASS
275	198	10	60	29.4	75987	PASS
365	198	1	100	4.4	11352	PASS
441	198	0.01	100	14.8	38339	PASS
442	442	50	100	100.0	229269	PASS
443	442	15	24	21.1	48312	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020224\
Data File : BG060535.D
Acq On : 1 Feb 2024 15:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 02 01:08:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

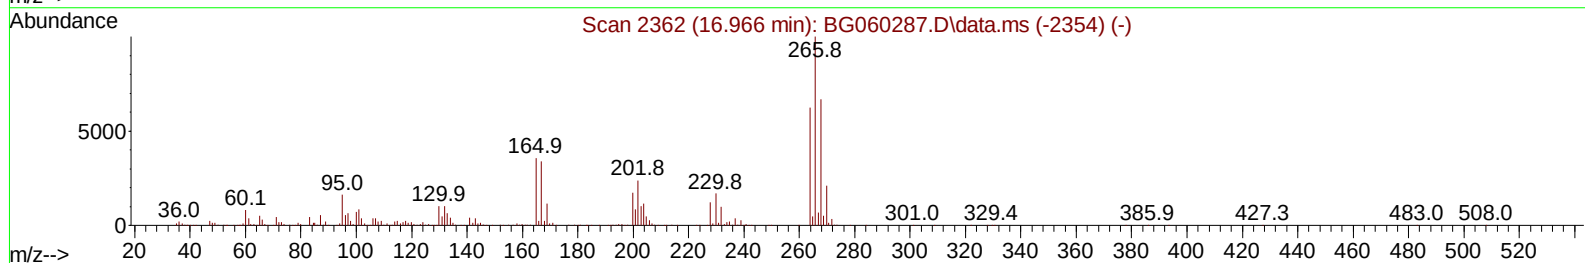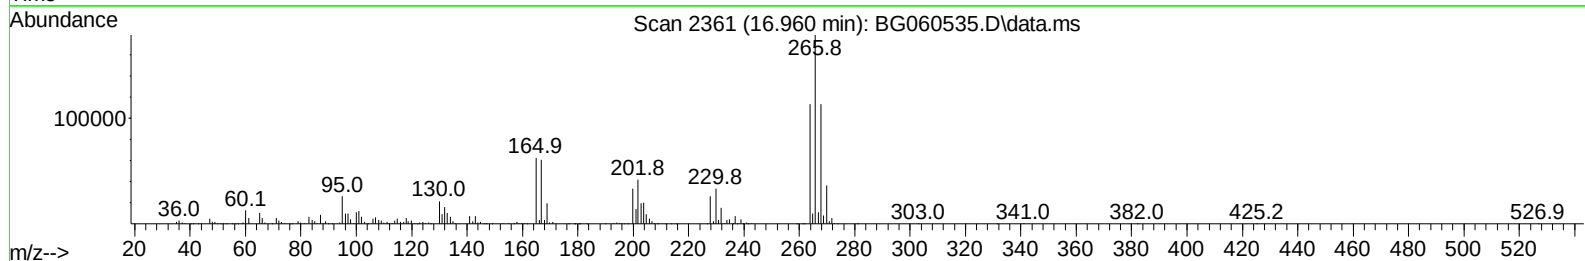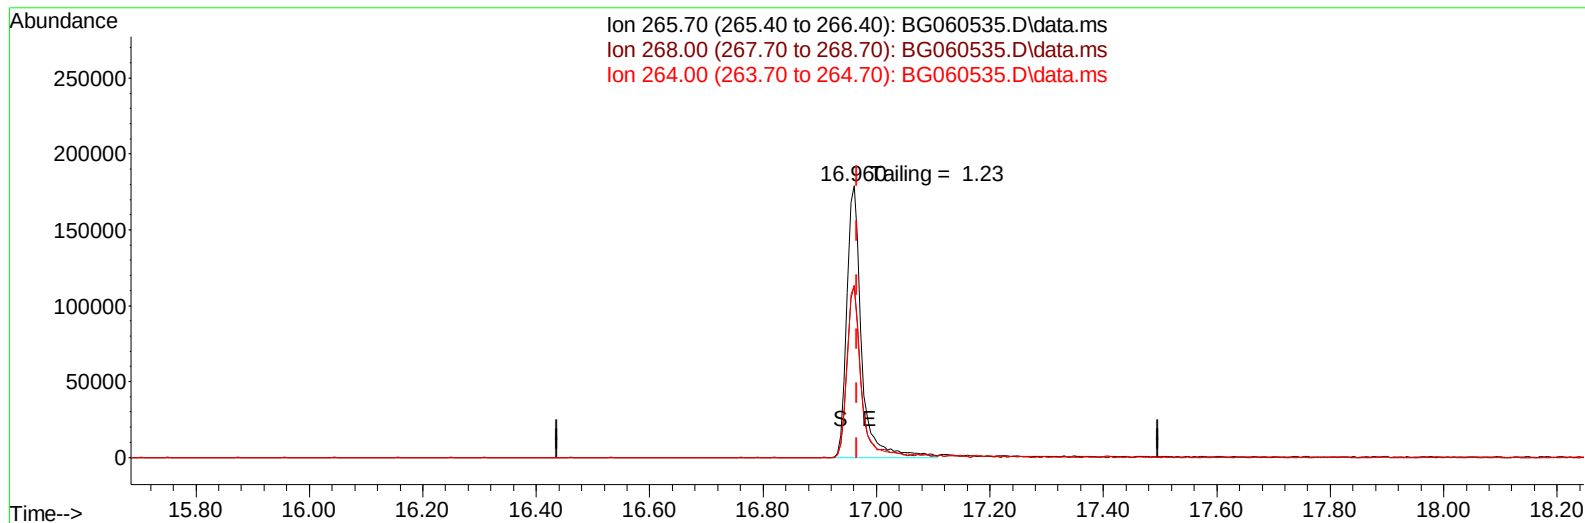

TIC: BG060535.D\data.ms

(70) Pentachlorophenol (C)

16.960min (-0.006) 798052.99 ng




response 324511

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	63.30
264.00	62.30	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020224\
Data File : BG060535.D
Acq On : 1 Feb 2024 15:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 02 01:08:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

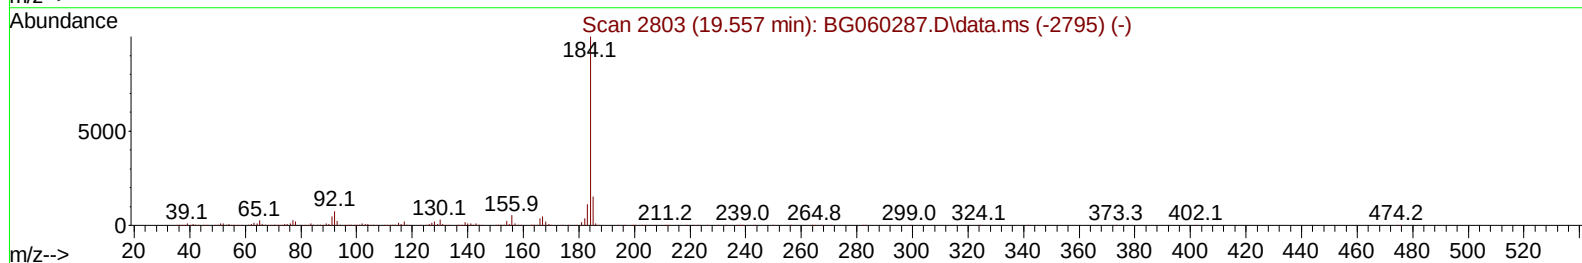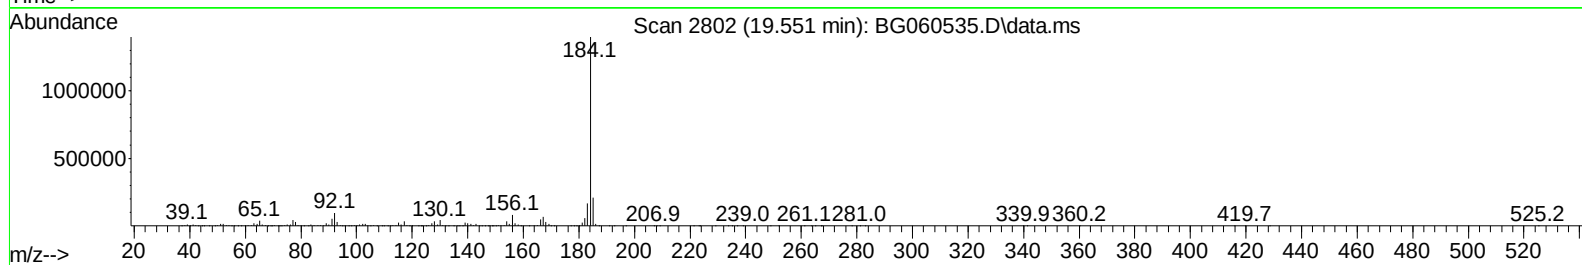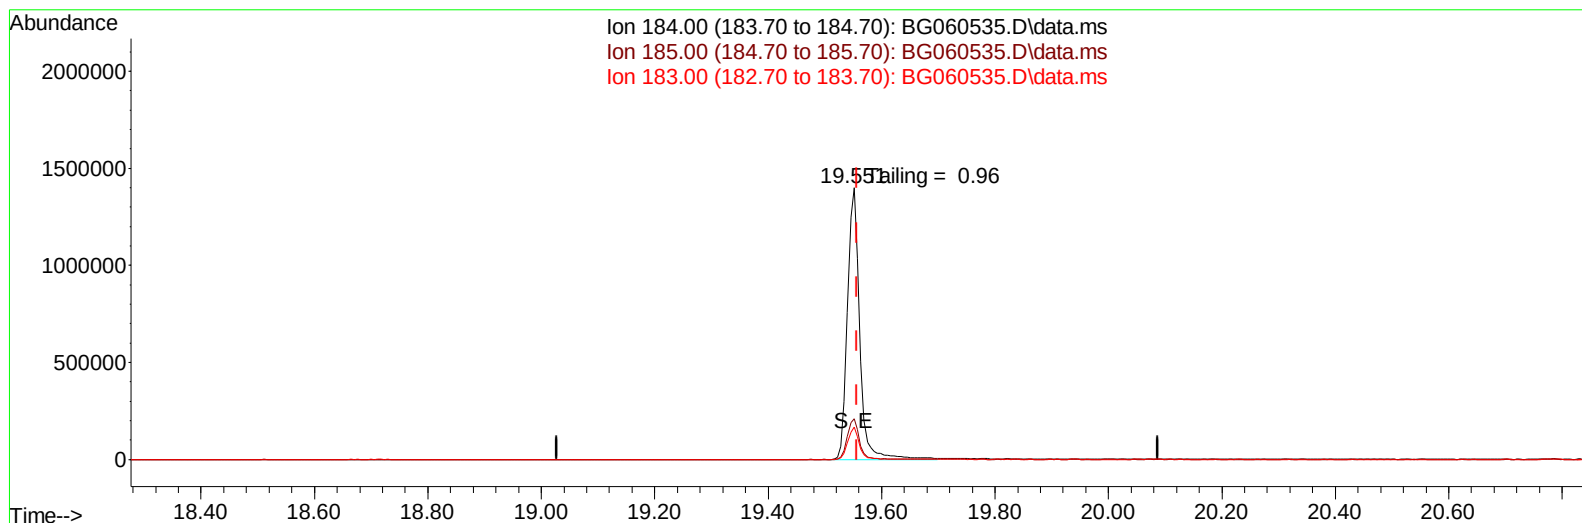

TIC: BG060535.D\data.ms

(77) Benzidine

19.551min (-0.006) 468842.84 ng

response 2118627

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	15.03
183.00	11.20	11.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/2/2024	BNA_G	<u>BG060535.D</u>
Compound Name	Response	Retention Time
DDT	996582	20.779
DDD	89299	20.339
DDE	1234	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
90533	1087115	8.33

Instrument :
BNA_G
ClientSampleId :
DFTPP