
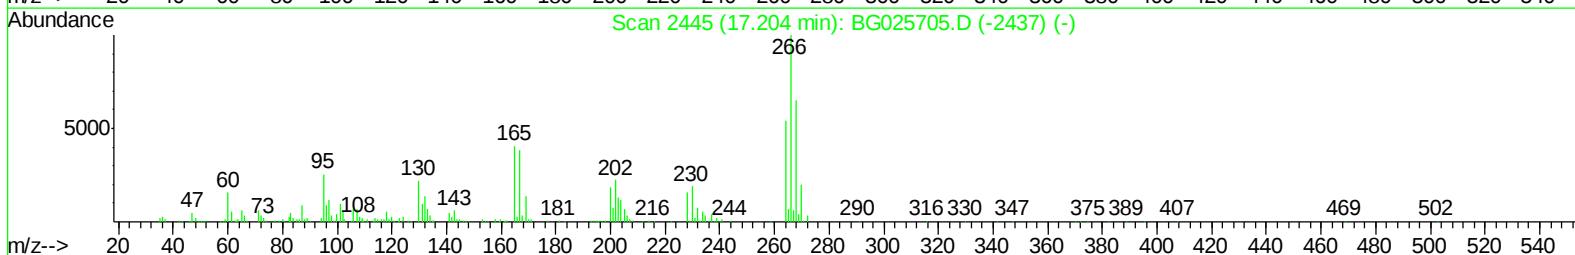
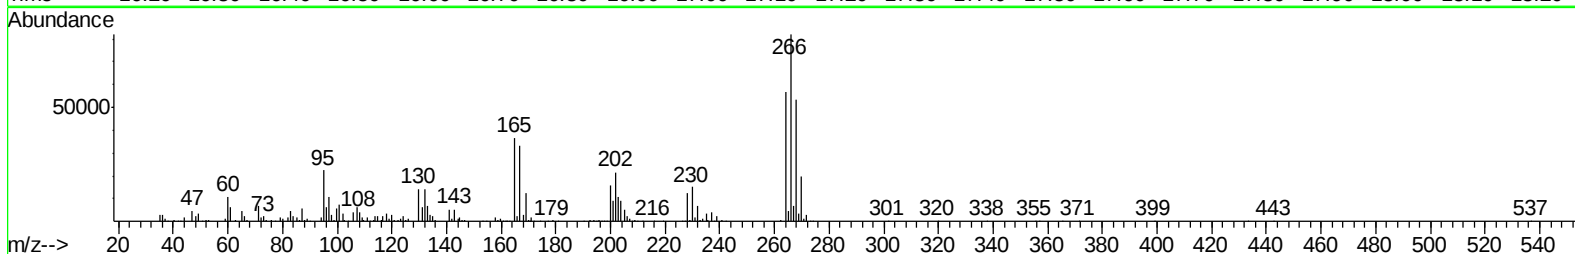


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020317\
Data File : BG025763.D
Acq On : 2 Feb 2017 18:22
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 06:33:07 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 18:29:38 2017
Response via : Initial Calibration

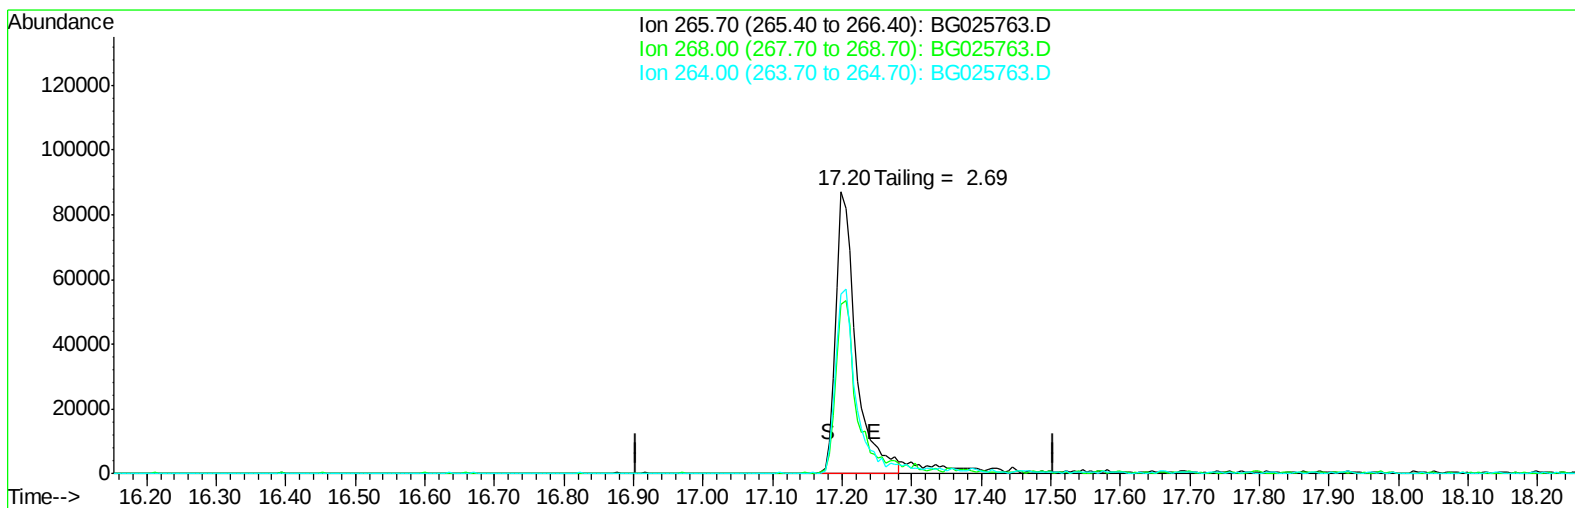

TIC: BG025763.D

(69) Pentachlorophenol (C)




17.204min (-17.204) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	60.70	0.00#
264.00	62.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020317\
 Data File : BG025763.D
 Acq On : 2 Feb 2017 18:22
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 06:33:07 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 30 18:29:38 2017
 Response via : Initial Calibration

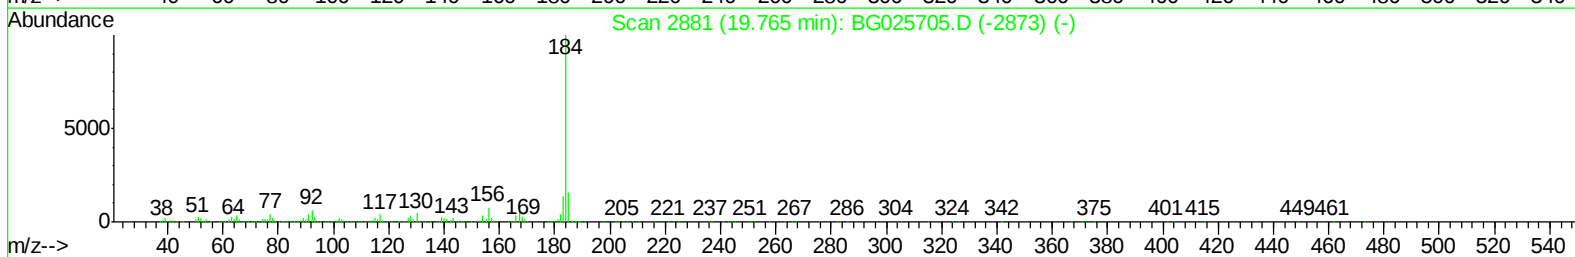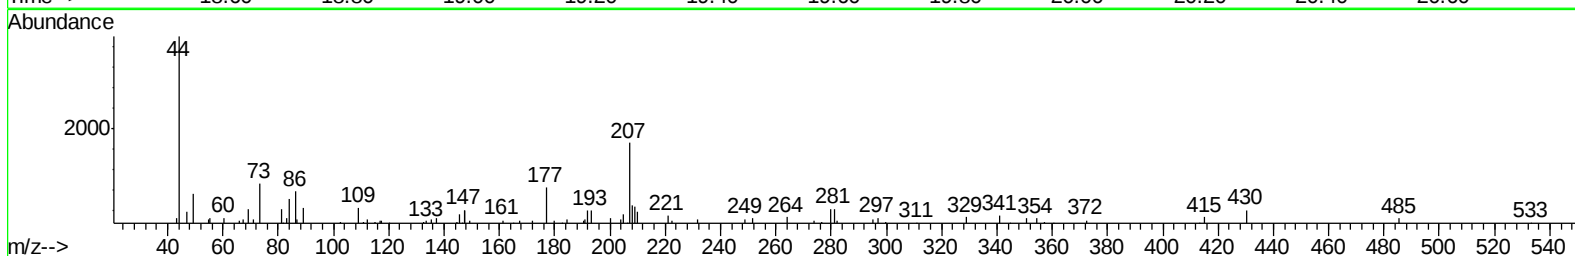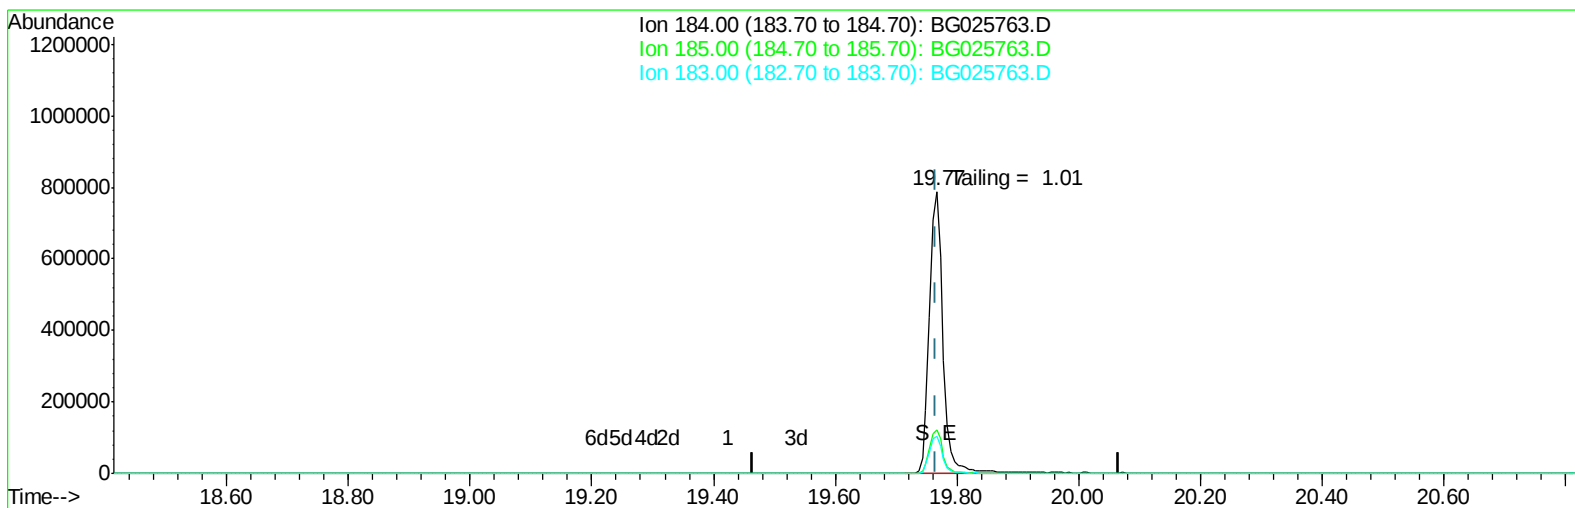

TIC: BG025763.D

(76) Benzidine

19.425min (-0.340) 10.03ng

response 84

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	0.00#
183.00	13.80	0.00#
0.00	0.00	0.00