
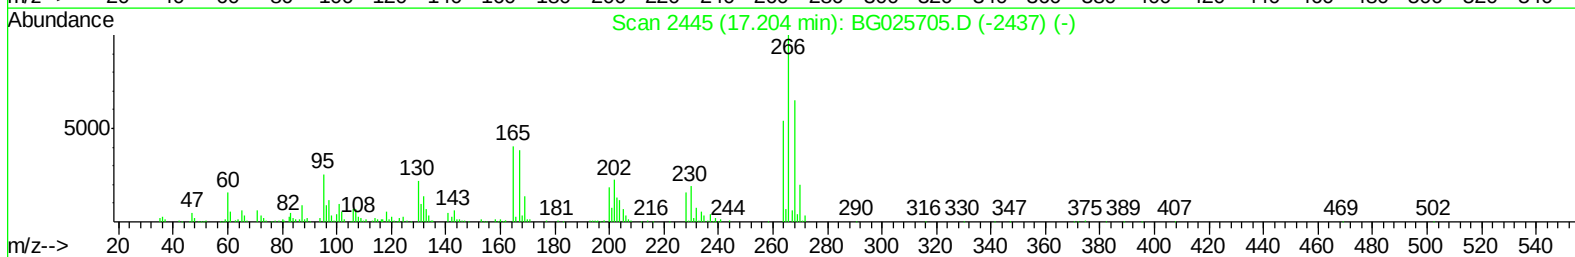
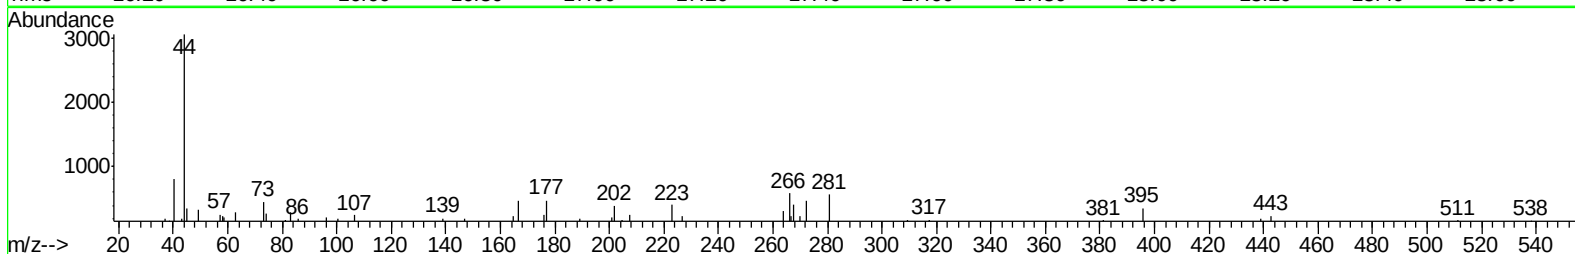


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020317\
 Data File : BG025781.D
 Acq On : 3 Feb 2017 6:06
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 07:09:22 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 30 18:29:38 2017
 Response via : Initial Calibration

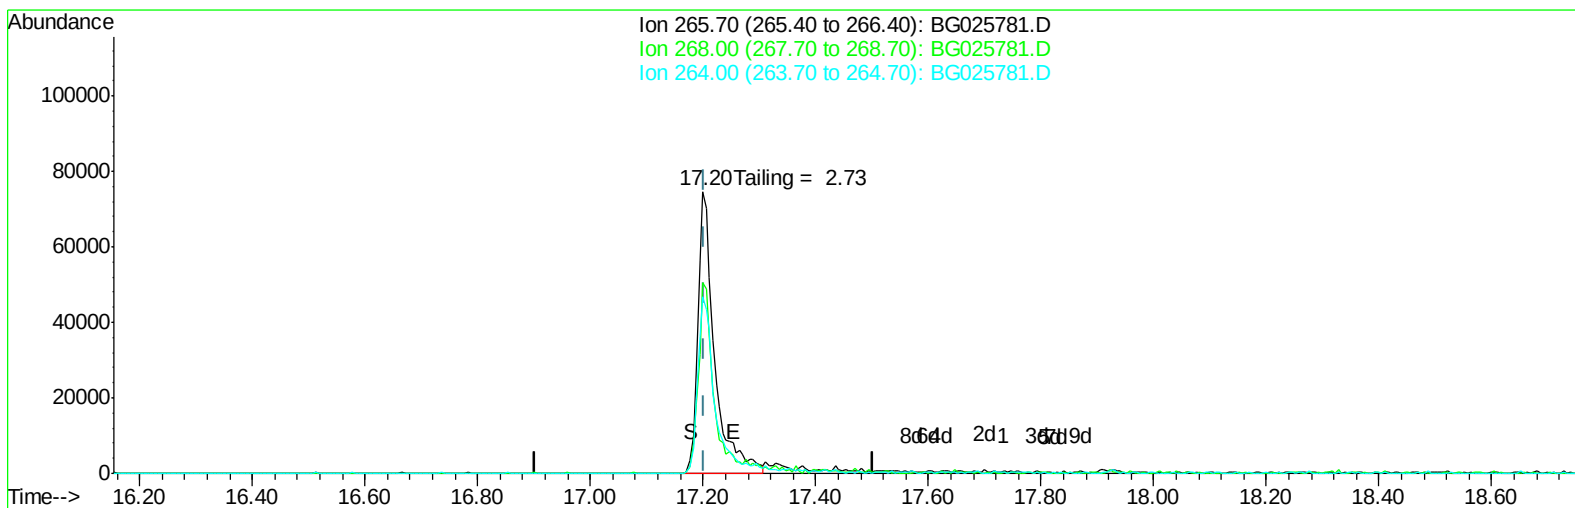

TIC: BG025781.D

(69) Pentachlorophenol (C)




17.735min (+0.531) 714.91ng

response 348

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	72.24
264.00	62.60	55.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020317\
 Data File : BG025781.D
 Acq On : 3 Feb 2017 6:06
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 03 07:09:22 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 30 18:29:38 2017
 Response via : Initial Calibration

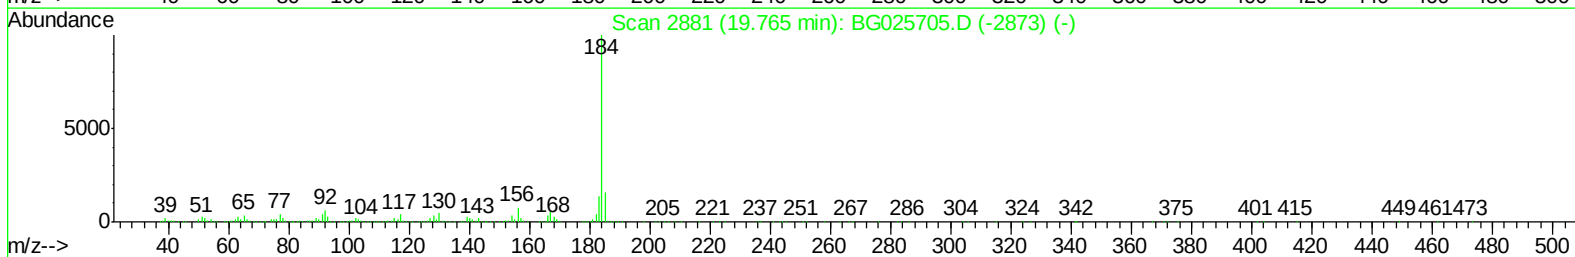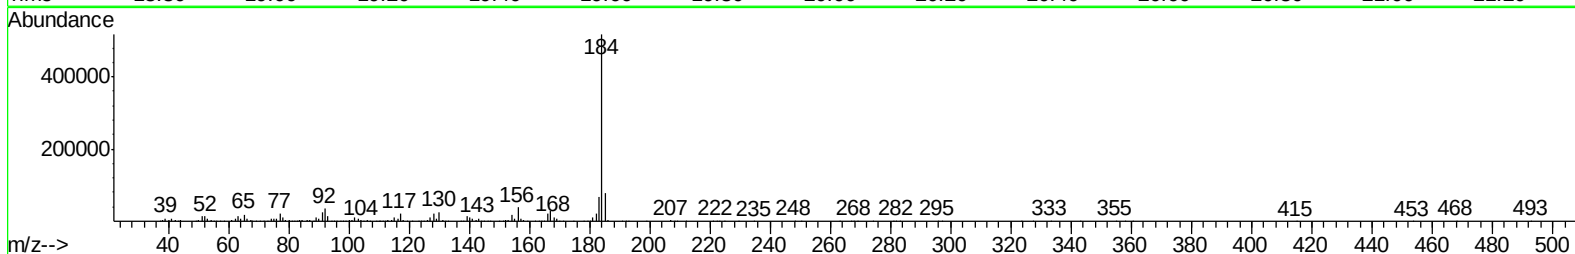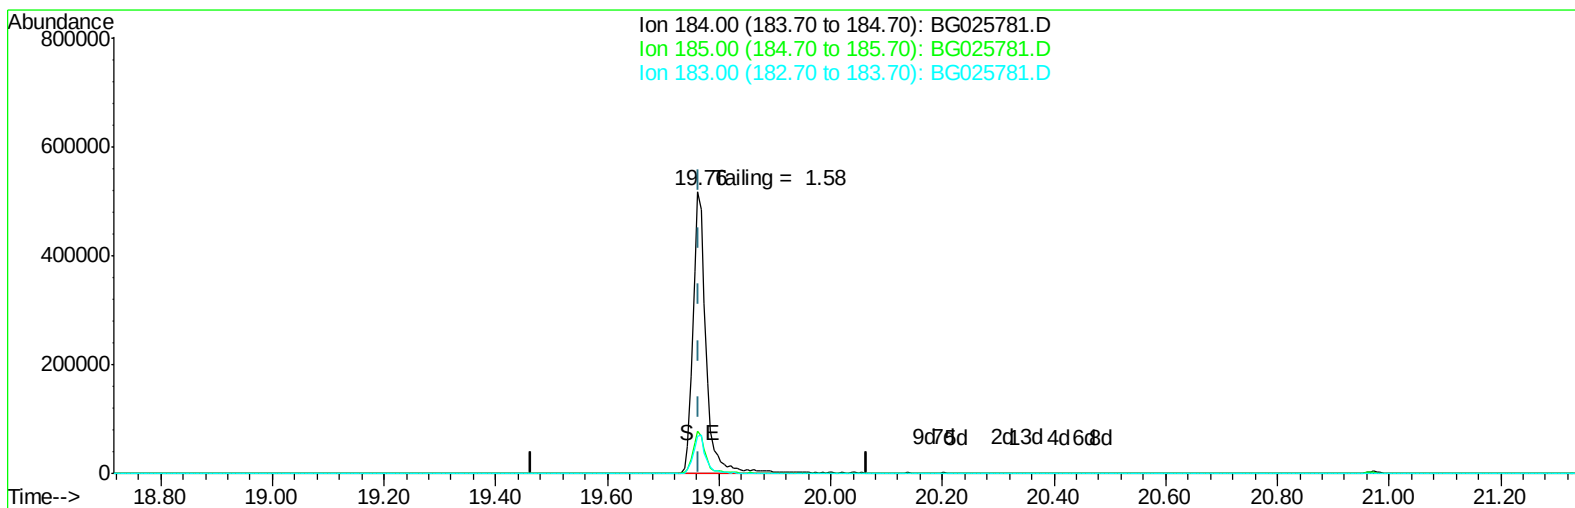

TIC: BG025781.D

(76) Benzidine

19.762min (-0.004) 186072.60ng m

response 843410

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.07
183.00	13.80	12.99
0.00	0.00	0.00