


Data Path : Z:\HPCHEM1\BNA G\DATA\BG020317\
 Data File : BG025781.D
 Acq On : 3 Feb 2017 6:06
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 18:29:38 2017

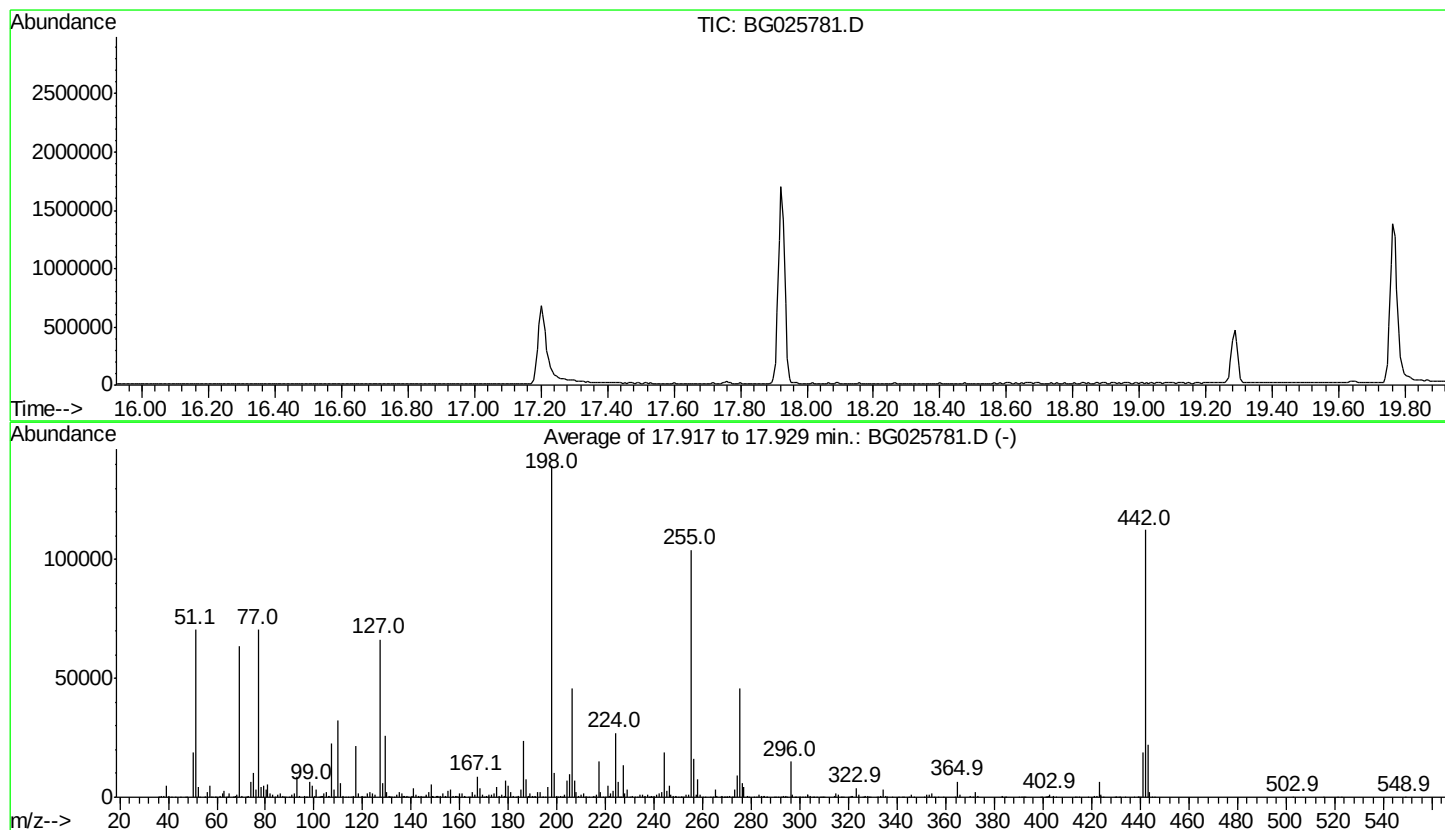

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.5	70432	PASS
68	69	0.00	2	1.7	1103	PASS
69	198	0.00	100	45.6	63650	PASS
70	69	0.00	2	0.6	392	PASS
127	198	10	80	47.6	66469	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	139573	PASS
199	198	5	9	7.5	10509	PASS
275	198	10	60	32.8	45736	PASS
365	198	1	100	4.8	6681	PASS
441	442	0.01	24	16.6	18690	PASS
442	198	50	100	80.6	112528	PASS
443	442	15	24	19.8	22327	PASS