

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
 Data File : BG048088.D
 Acq On : 3 Feb 2021 12:22
 Operator : CG/JU
 Sample : M1292-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU421-009-1015

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048088.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.673	390	397	409	rVB	595337	945012	4.84%	1.485%
2	7.265	659	668	678	rBV	613822	1034297	5.29%	1.625%
3	8.117	806	813	819	rBV	166838	268336	1.37%	0.422%
4	9.281	1003	1011	1018	rBV	352707	634578	3.25%	0.997%
5	10.932	1284	1292	1299	rBV	198227	356585	1.83%	0.560%
6	13.364	1700	1706	1713	rBV	899753	1383106	7.08%	2.173%
7	14.739	1934	1940	1946	rBV	328188	509808	2.61%	0.801%
8	16.220	2186	2192	2204	rBV	864098	1448796	7.42%	2.277%
9	17.483	2402	2407	2413	rVB	497930	717709	3.67%	1.128%
10	18.352	2550	2555	2568	rVB2	842277	1990870	10.19%	3.128%
11	18.770	2609	2626	2636	rBV	1789753	7373046	37.74%	11.586%
12	18.911	2636	2650	2659	rVV	2311028	9205243	47.12%	14.465%
13	19.040	2659	2672	2679	rVB	6024342	19536553	100.00%	30.699%
14	19.175	2688	2695	2705	rVB	700604	1528630	7.82%	2.402%
15	19.616	2756	2770	2789	rVB2	1283044	4424445	22.65%	6.952%
16	19.909	2814	2820	2829	rVB	576516	1024485	5.24%	1.610%
17	20.086	2844	2850	2855	rVB	2165153	2838669	14.53%	4.461%
18	20.708	2950	2956	2963	rBV	788299	1354247	6.93%	2.128%
19	21.396	3068	3073	3079	rBV3	176199	326635	1.67%	0.513%
20	21.496	3081	3090	3099	rVB2	666944	1551844	7.94%	2.438%
21	21.754	3128	3134	3140	rVB2	572864	913252	4.67%	1.435%
22	22.383	3234	3241	3251	rBV	564045	1309380	6.70%	2.057%
23	23.417	3410	3417	3427	rVB2	388592	1026125	5.25%	1.612%
24	24.622	3614	3622	3634	rVB3	312975	977268	5.00%	1.536%
25	25.033	3685	3692	3706	rVB2	320914	960980	4.92%	1.510%




Sum of corrected areas: 63639899

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048088.D
Acq On : 3 Feb 2021 12:22
Operator : CG/JU
Sample : M1292-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU421-009-1015

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

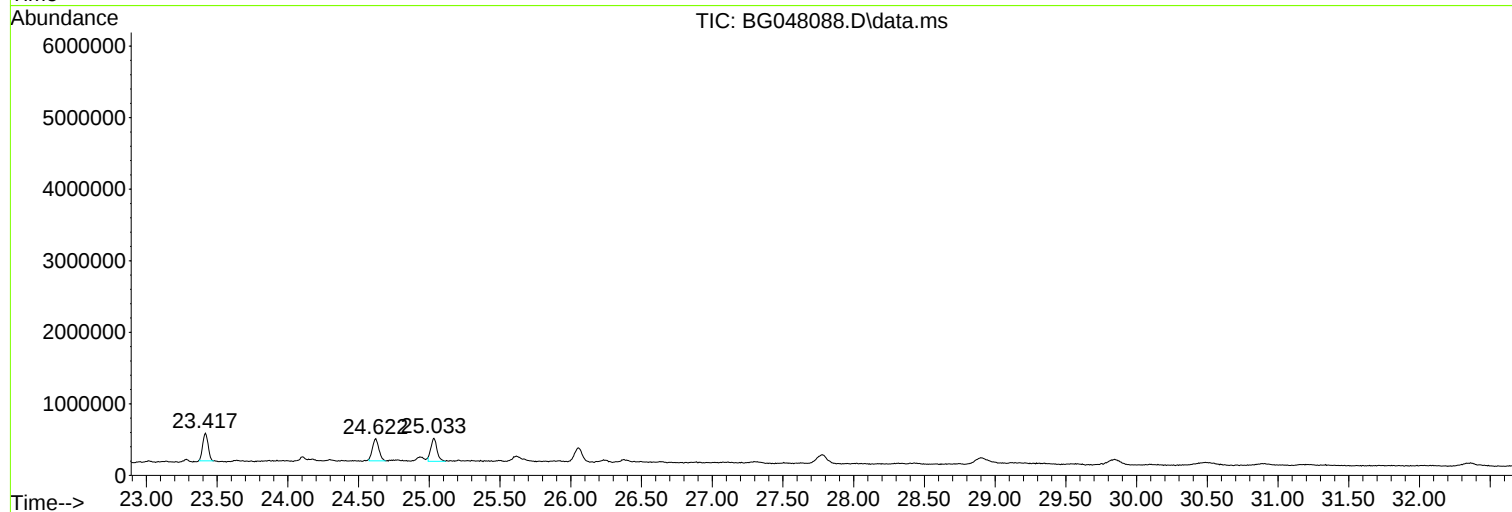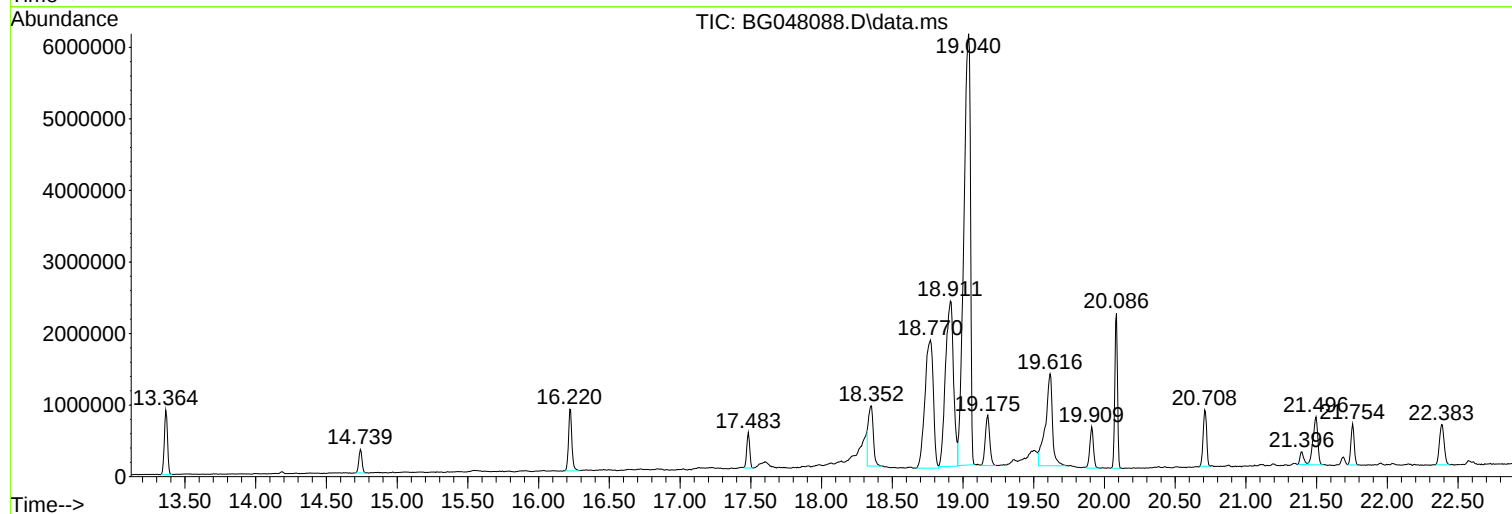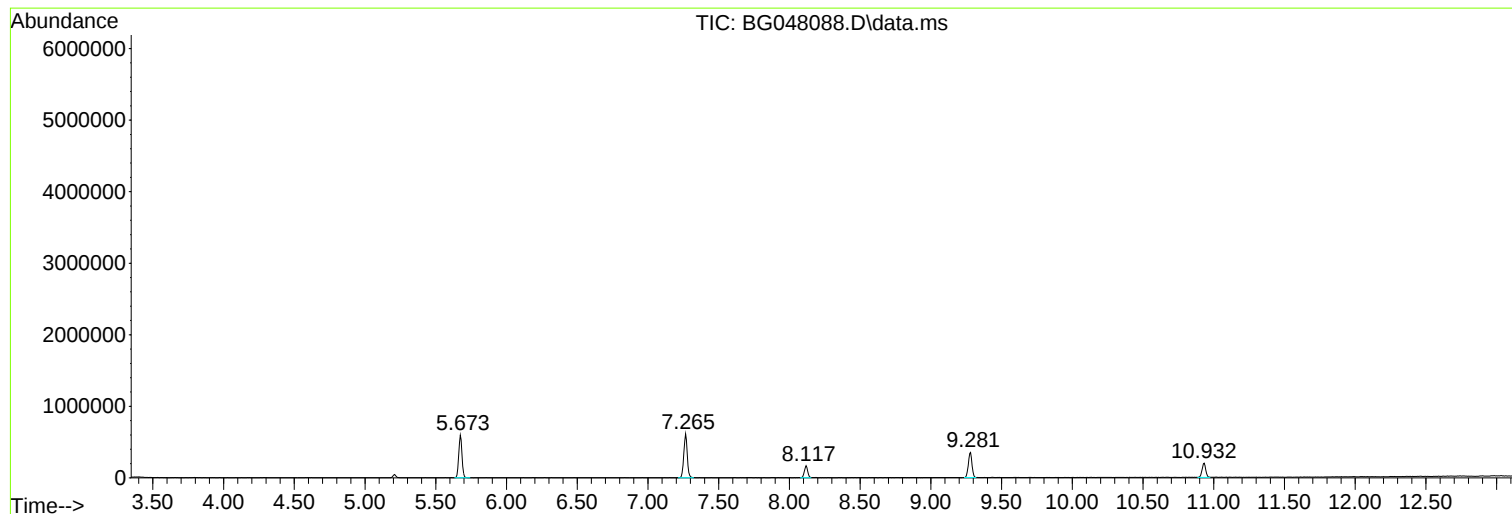

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048088.D
Acq On : 3 Feb 2021 12:22
Operator : CG/JU
Sample : M1292-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU421-009-1015

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048088.D
Acq On : 3 Feb 2021 12:22
Operator : CG/JU
Sample : M1292-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU421-009-1015

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------