

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
 Data File : BG048098.D
 Acq On : 3 Feb 2021 19:37
 Operator : CG/JU
 Sample : M1291-20
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 2021-01-27-EB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048098.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.670	387	397	404	rBV	526315	822449	17.87%	4.031%
2	6.152	468	479	480	rBV2	66527	102154	2.22%	0.501%
3	6.176	480	483	489	rVB	125715	187386	4.07%	0.918%
4	7.263	661	668	678	rVB2	313661	639129	13.88%	3.133%
5	8.115	806	813	818	rBV	172993	285547	6.20%	1.400%
6	8.167	818	822	831	rVB2	32017	52199	1.13%	0.256%
7	8.344	846	852	861	rBV2	71430	127203	2.76%	0.623%
8	9.213	991	1000	1004	rBV	104010	173975	3.78%	0.853%
9	9.278	1004	1011	1019	rVB	604203	1078103	23.42%	5.284%
10	9.437	1032	1038	1047	rVB	183484	288512	6.27%	1.414%
11	10.159	1154	1161	1168	rBV5	57974	134134	2.91%	0.657%
12	10.388	1195	1200	1206	rBV3	29288	51393	1.12%	0.252%
13	10.929	1284	1292	1305	rBV2	227920	485588	10.55%	2.380%
14	13.103	1656	1662	1669	rBV	98496	153740	3.34%	0.754%
15	13.361	1697	1706	1713	rBV	1614530	2643869	57.43%	12.958%
16	13.649	1747	1755	1764	rBV	93348	162736	3.53%	0.798%
17	13.843	1781	1788	1798	rBV	112444	223822	4.86%	1.097%
18	14.178	1841	1845	1850	rBV	33201	55023	1.20%	0.270%
19	14.736	1934	1940	1948	rVB	392705	603872	13.12%	2.960%
20	15.541	2069	2077	2081	rBV2	48163	78590	1.71%	0.385%
21	16.217	2185	2192	2207	rBV	1464449	2303567	50.04%	11.290%
22	17.480	2397	2407	2415	rBV	558421	815354	17.71%	3.996%
23	18.138	2514	2519	2529	rBV	397227	538832	11.70%	2.641%
24	18.361	2551	2557	2568	rBV	478569	743888	16.16%	3.646%
25	19.489	2744	2749	2752	rBV3	30496	48877	1.06%	0.240%
26	19.625	2768	2772	2784	rBV	339095	514431	11.17%	2.521%
27	20.083	2844	2850	2856	rBV	3596940	4603681	100.00%	22.564%
28	21.387	3067	3072	3082	rBV	171515	302840	6.58%	1.484%
29	21.752	3128	3134	3142	rVB	564505	934612	20.30%	4.581%
30	24.102	3530	3534	3541	rVB2	52446	95186	2.07%	0.467%
31	25.030	3682	3692	3709	rVB2	323849	1053838	22.89%	5.165%
32	26.229	3889	3896	3907	rVB4	34314	98584	2.14%	0.483%




Sum of corrected areas: 20403114

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048098.D
Acq On : 3 Feb 2021 19:37
Operator : CG/JU
Sample : M1291-20
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
2021-01-27-EB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

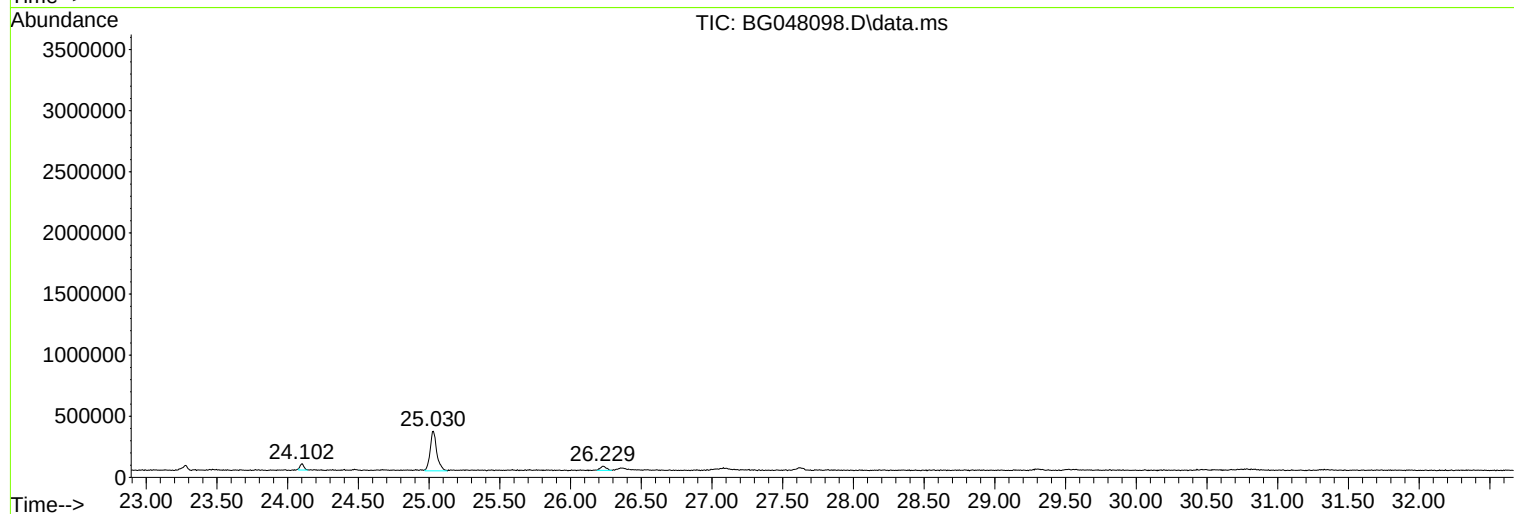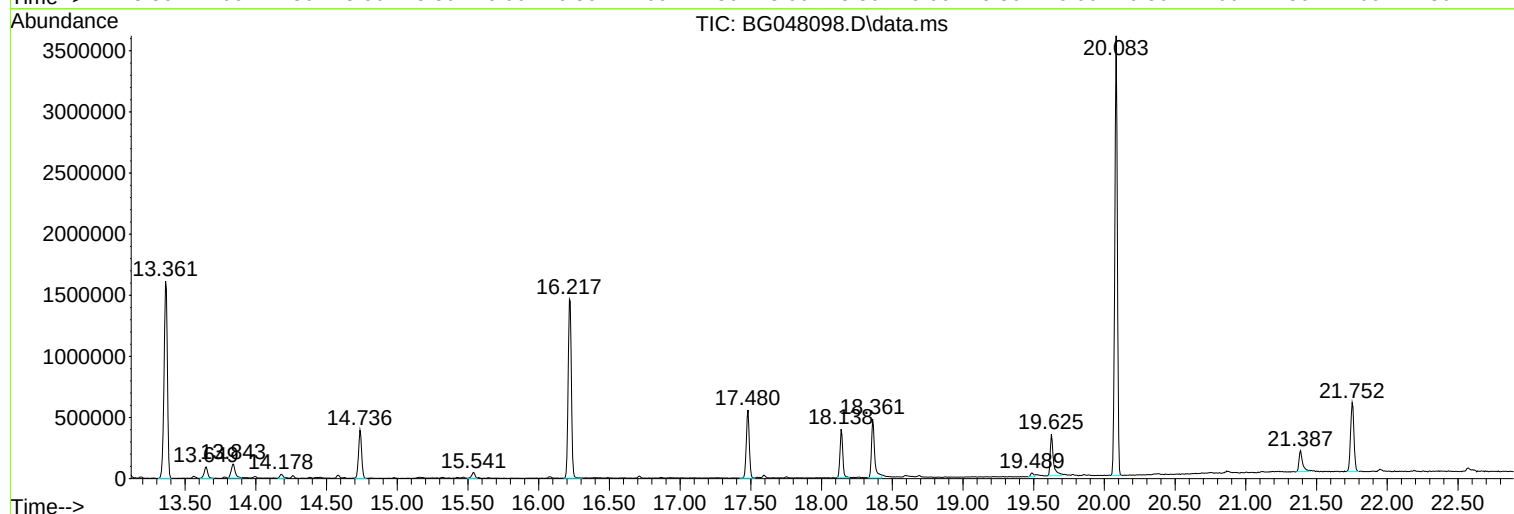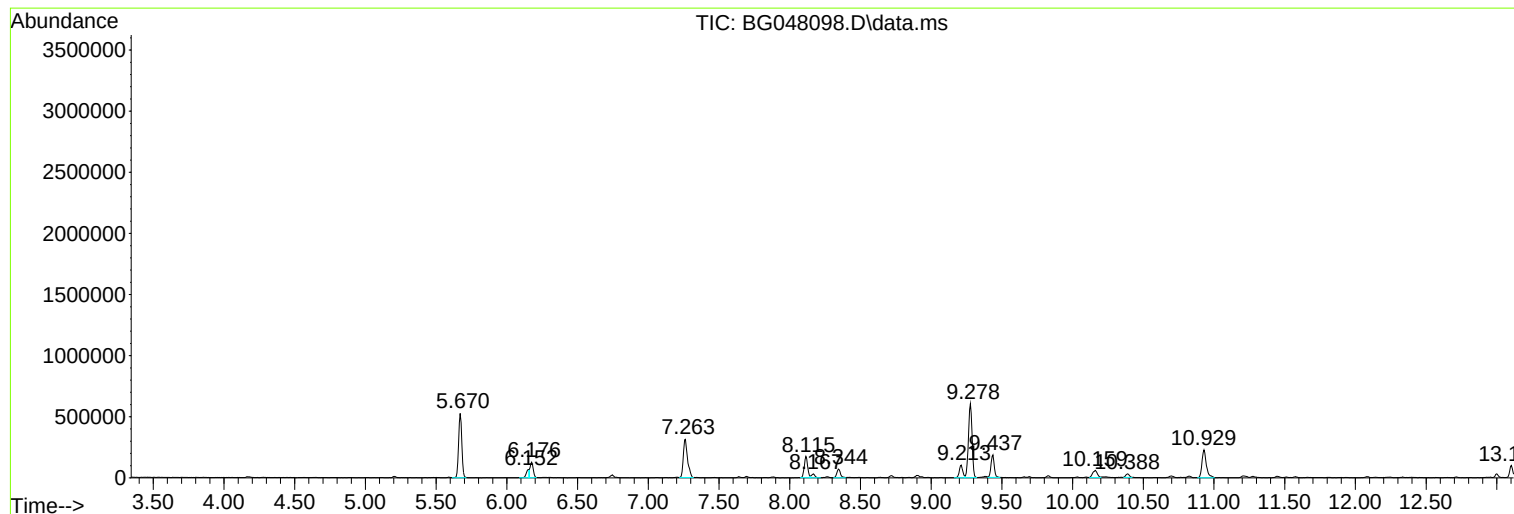

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048098.D
Acq On : 3 Feb 2021 19:37
Operator : CG/JU
Sample : M1291-20
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
2021-01-27-EB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048098.D
Acq On : 3 Feb 2021 19:37
Operator : CG/JU
Sample : M1291-20
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
2021-01-27-EB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------