

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
 Data File : BG048099.D
 Acq On : 3 Feb 2021 20:17
 Operator : CG/JU
 Sample : M1292-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 2021-01-28-EB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.670	389	397	407	rVB	519862	815437	17.50%	3.984%
2	6.175	472	483	490	rBV2	129583	287029	6.16%	1.402%
3	7.262	661	668	679	rVB2	312892	639835	13.73%	3.126%
4	8.114	807	813	818	rBV	174355	288687	6.19%	1.410%
5	8.167	818	822	827	rVB4	30566	49265	1.06%	0.241%
6	8.344	843	852	862	rBV2	69524	124512	2.67%	0.608%
7	9.213	993	1000	1005	rBV2	97875	176035	3.78%	0.860%
8	9.278	1005	1011	1019	rVB	632109	1082869	23.23%	5.290%
9	9.436	1032	1038	1050	rVB	173105	289988	6.22%	1.417%
10	10.159	1154	1161	1169	rBV3	55307	129394	2.78%	0.632%
11	10.388	1195	1200	1207	rBV2	28956	49573	1.06%	0.242%
12	10.929	1283	1292	1305	rBV2	230381	495978	10.64%	2.423%
13	13.103	1656	1662	1672	rBV	97227	160818	3.45%	0.786%
14	13.361	1697	1706	1716	rVB	1588894	2662483	57.13%	13.008%
15	13.649	1747	1755	1767	rBV2	88656	156889	3.37%	0.766%
16	13.843	1781	1788	1796	rBV	109051	203816	4.37%	0.996%
17	14.184	1841	1846	1855	rBV2	24744	46943	1.01%	0.229%
18	14.736	1934	1940	1948	rVB	394956	616958	13.24%	3.014%
19	15.541	2070	2077	2082	rBV2	45326	69956	1.50%	0.342%
20	16.223	2185	2193	2200	rBV	1551886	2357469	50.58%	11.517%
21	17.480	2400	2407	2415	rBV	558330	833042	17.87%	4.070%
22	18.138	2514	2519	2526	rBV	412386	536045	11.50%	2.619%
23	18.361	2552	2557	2567	rBV	483267	716485	15.37%	3.500%
24	19.489	2744	2749	2752	rBV6	30538	50298	1.08%	0.246%
25	19.624	2768	2772	2783	rBV	348515	506757	10.87%	2.476%
26	20.083	2844	2850	2856	rBV	3573397	4660706	100.00%	22.770%
27	21.387	3067	3072	3084	rBV3	185245	340811	7.31%	1.665%
28	21.751	3128	3134	3143	rVB	571241	961446	20.63%	4.697%
29	22.574	3270	3274	3279	rBV5	35070	59672	1.28%	0.292%
30	24.102	3530	3534	3539	rVB5	41822	74297	1.59%	0.363%
31	25.030	3682	3692	3707	rVB2	324944	1025192	22.00%	5.009%




Sum of corrected areas: 20468685

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048099.D
Acq On : 3 Feb 2021 20:17
Operator : CG/JU
Sample : M1292-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
2021-01-28-EB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

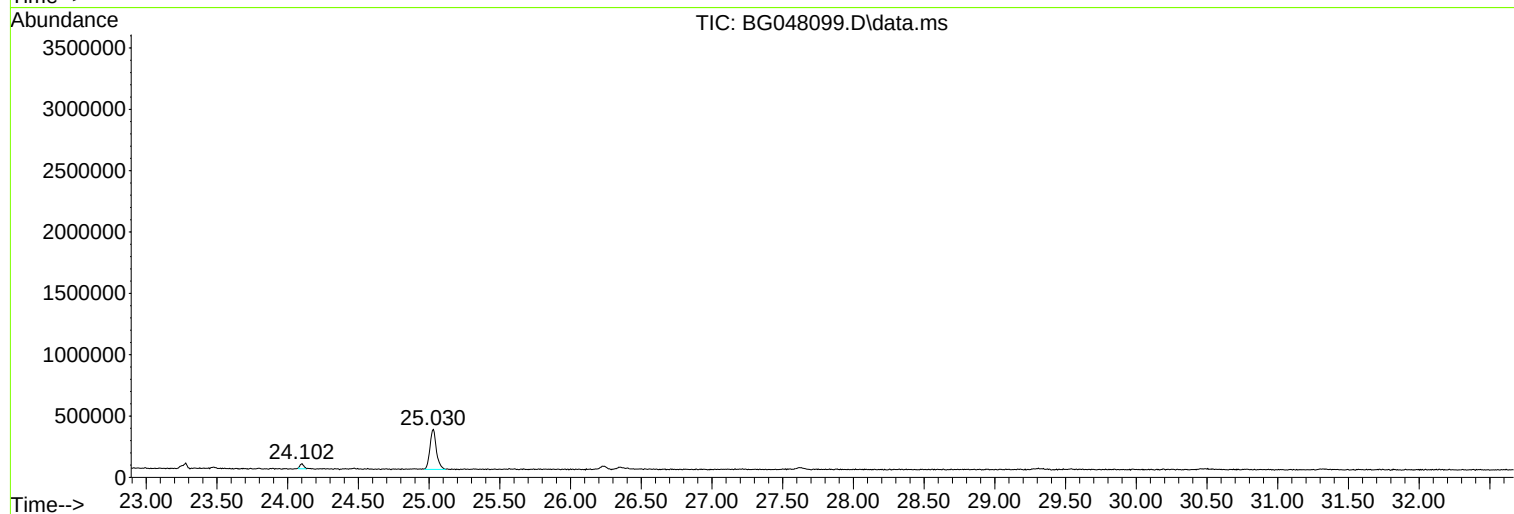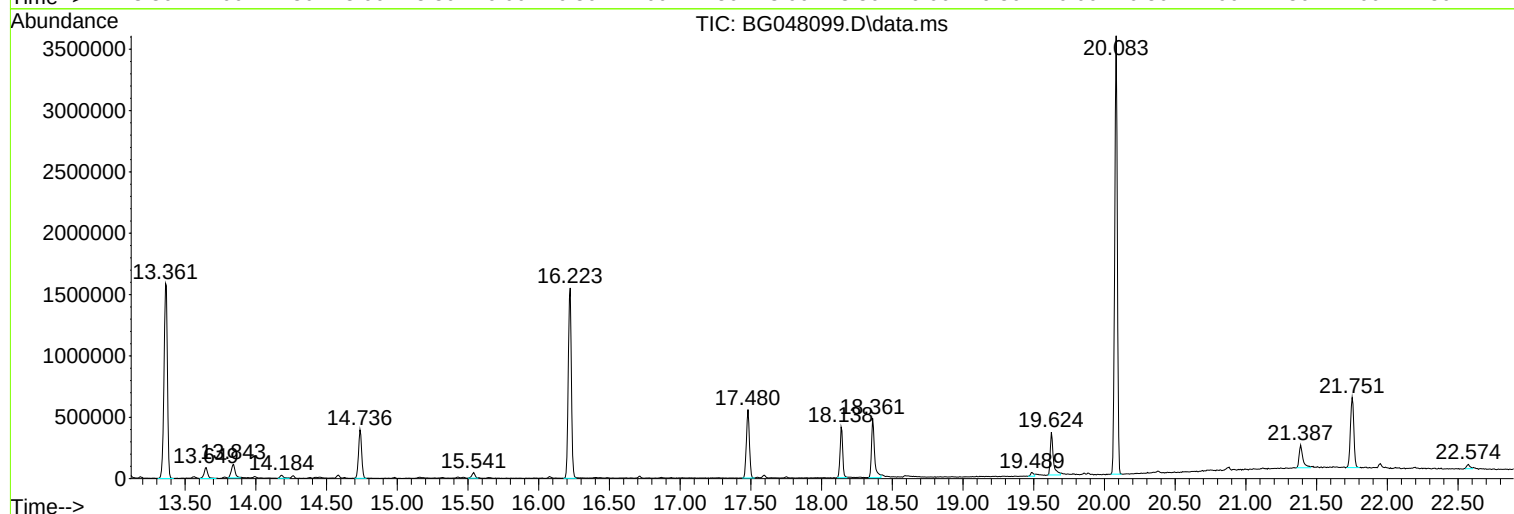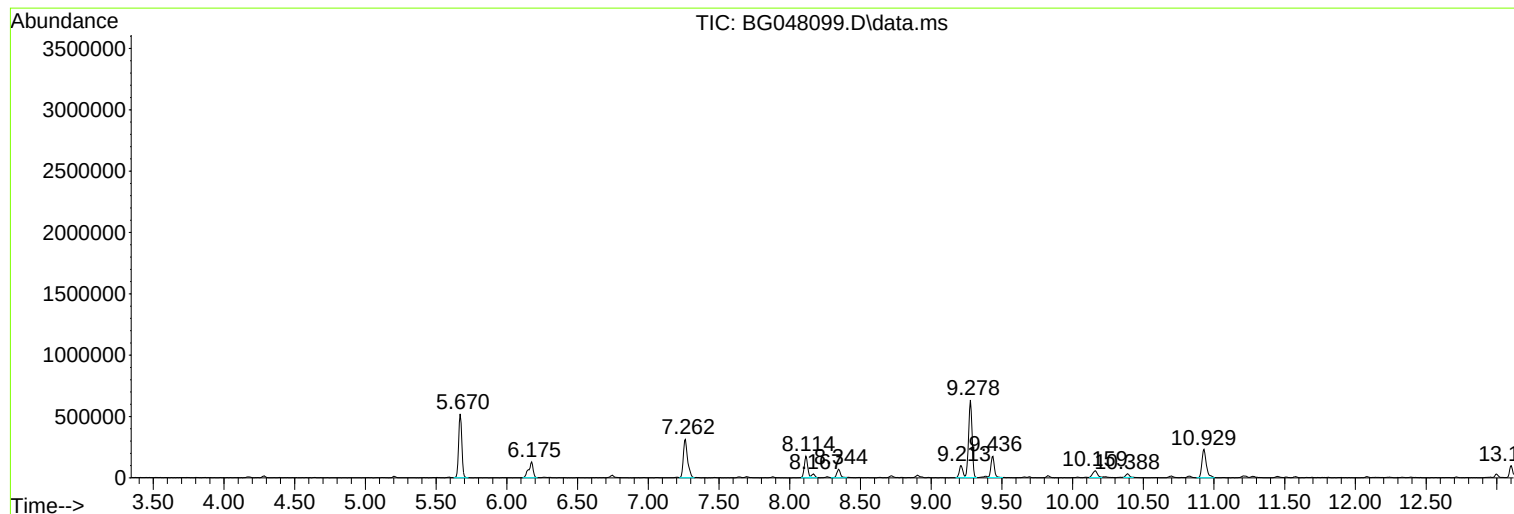

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048099.D
Acq On : 3 Feb 2021 20:17
Operator : CG/JU
Sample : M1292-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
2021-01-28-EB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048099.D
Acq On : 3 Feb 2021 20:17
Operator : CG/JU
Sample : M1292-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
2021-01-28-EB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------