

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
 Data File : BG048102.D
 Acq On : 3 Feb 2021 22:18
 Operator : CG/JU
 Sample : M1291-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU421-006-1015

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.668	389	396	406	rBV	711921	1122763	39.25%	8.044%
2	7.260	659	667	678	rBV	723236	1248716	43.65%	8.946%
3	8.118	803	813	820	rBV	167513	289931	10.14%	2.077%
4	9.275	1000	1010	1018	rBV	439008	764008	26.71%	5.473%
5	10.926	1282	1291	1299	rBV	226539	396304	13.85%	2.839%
6	13.359	1698	1705	1713	rBV	1093850	1736104	60.69%	12.438%
7	14.181	1839	1845	1852	rBV2	29462	41652	1.46%	0.298%
8	14.734	1930	1939	1946	rBV	377515	611189	21.37%	4.379%
9	16.220	2185	2192	2204	rBV	1075266	1567306	54.79%	11.228%
10	17.477	2400	2406	2412	rBV	563389	820811	28.69%	5.880%
11	18.359	2551	2556	2567	rBV2	127756	222235	7.77%	1.592%
12	19.628	2767	2772	2784	rBV4	62131	136340	4.77%	0.977%
13	20.080	2843	2849	2857	rBV	2291404	2860495	100.00%	20.493%
14	21.385	3067	3071	3081	rBV4	77471	137648	4.81%	0.986%
15	21.755	3127	3134	3142	rBV	566212	941329	32.91%	6.744%
16	23.253	3384	3389	3398	rVB10	24699	68107	2.38%	0.488%
17	24.099	3528	3533	3539	rVB7	16337	33500	1.17%	0.240%
18	25.027	3682	3691	3707	rVB2	326761	960165	33.57%	6.879%




Sum of corrected areas: 13958603

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048102.D
Acq On : 3 Feb 2021 22:18
Operator : CG/JU
Sample : M1291-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU421-006-1015

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

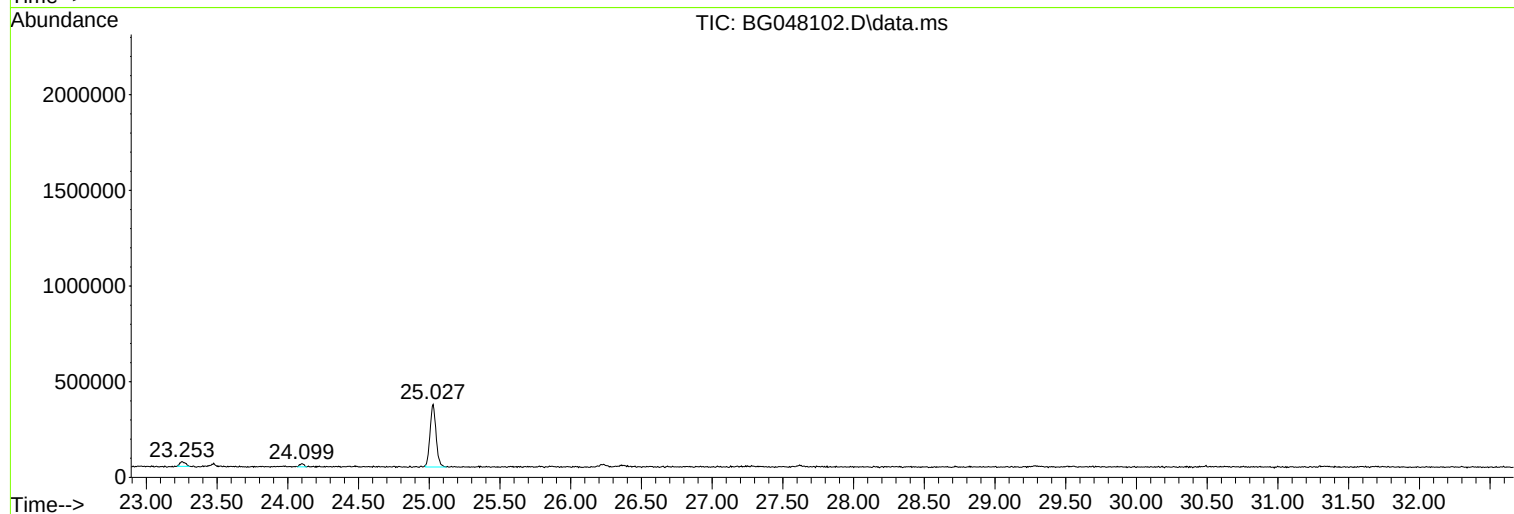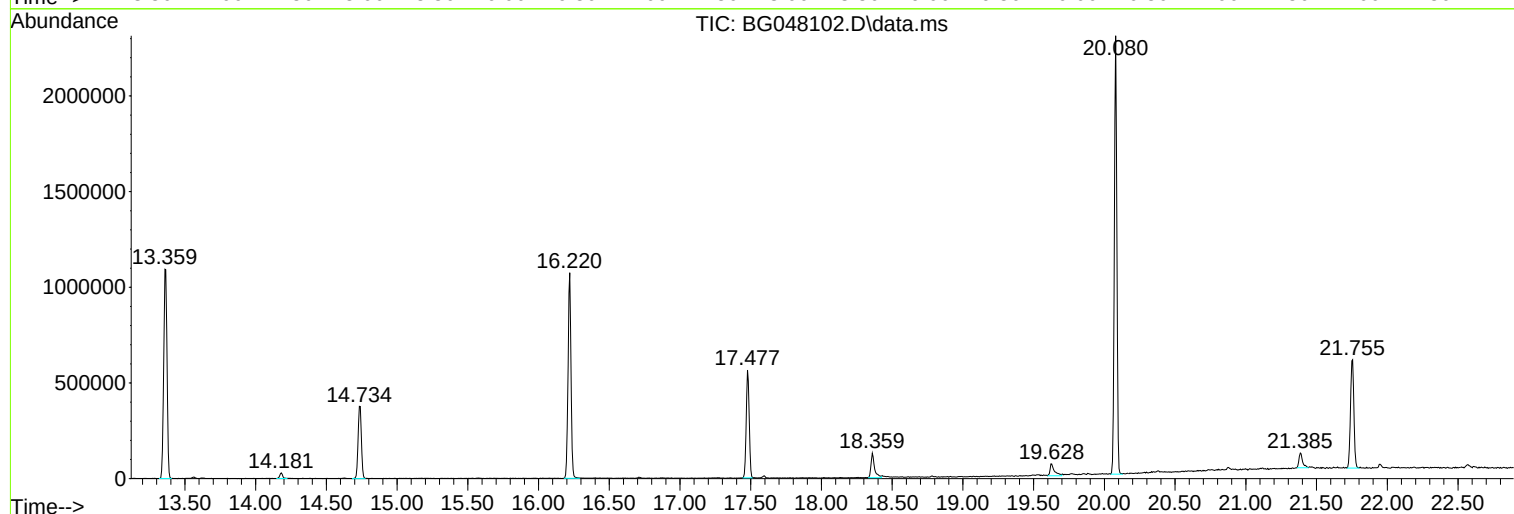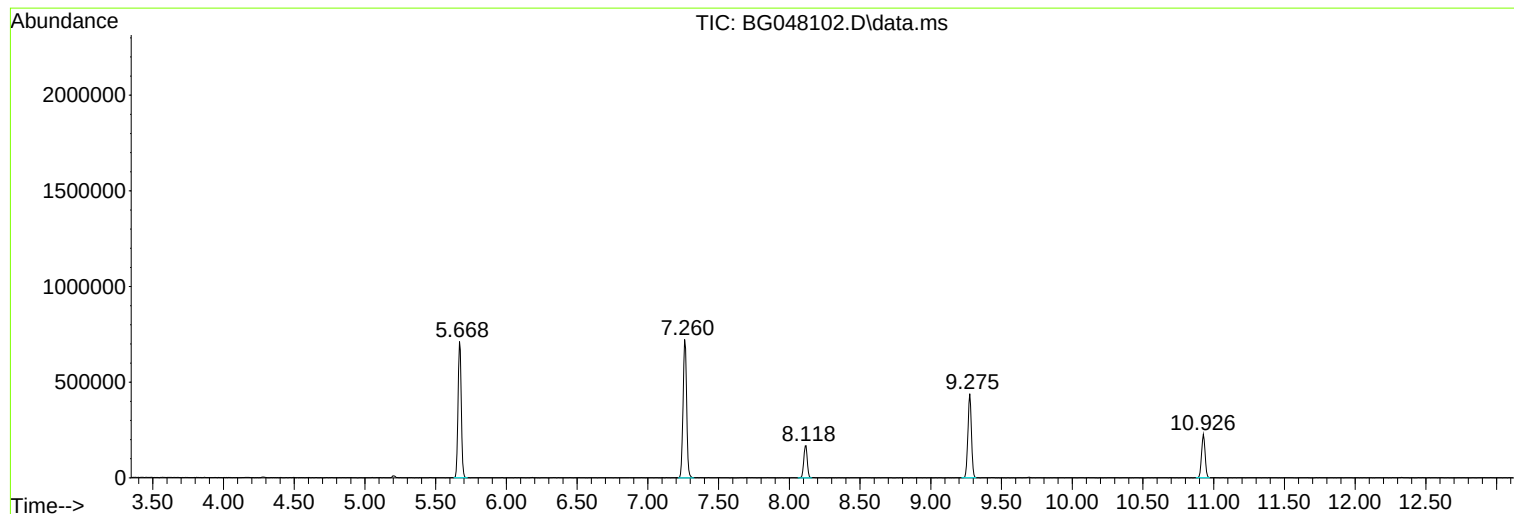

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048102.D
Acq On : 3 Feb 2021 22:18
Operator : CG/JU
Sample : M1291-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU421-006-1015

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048102.D
Acq On : 3 Feb 2021 22:18
Operator : CG/JU
Sample : M1291-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU421-006-1015

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
