

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
 Data File : BG048103.D
 Acq On : 3 Feb 2021 22:59
 Operator : CG/JU
 Sample : M1291-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU421-007-1015

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.671	390	397	407	rBV	781255	1215072	39.96%	8.216%
2	7.263	660	668	676	rBV	783708	1343864	44.19%	9.087%
3	8.115	806	813	820	rBV	167705	278667	9.16%	1.884%
4	9.273	1000	1010	1020	rBV	462842	835023	27.46%	5.646%
5	10.924	1283	1291	1303	rBV	219271	392644	12.91%	2.655%
6	13.362	1699	1706	1714	rBV	1238044	1874399	61.64%	12.674%
7	14.179	1841	1845	1856	rVB2	27726	45322	1.49%	0.306%
8	14.737	1933	1940	1948	rVB2	399644	615220	20.23%	4.160%
9	16.218	2185	2192	2204	rBV	1143107	1697088	55.81%	11.475%
10	17.481	2396	2407	2415	rBV	553047	816900	26.86%	5.524%
11	18.356	2550	2556	2570	rBV	140524	247253	8.13%	1.672%
12	19.625	2768	2772	2777	rBV2	60456	90729	2.98%	0.613%
13	20.078	2843	2849	2855	rBV	2324281	3040932	100.00%	20.562%
14	20.877	2982	2985	2989	rVB5	25432	31160	1.02%	0.211%
15	21.382	3067	3071	3081	rBV	156572	262243	8.62%	1.773%
16	21.752	3128	3134	3140	rVB	574350	908041	29.86%	6.140%
17	21.946	3163	3167	3172	rBV5	32003	48419	1.59%	0.327%
18	22.569	3268	3273	3277	rBV4	32905	60609	1.99%	0.410%
19	24.097	3531	3533	3540	rVB6	24812	35813	1.18%	0.242%
20	25.025	3682	3691	3706	rVB2	318829	949526	31.22%	6.421%




Sum of corrected areas: 14788924

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048103.D
Acq On : 3 Feb 2021 22:59
Operator : CG/JU
Sample : M1291-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU421-007-1015

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

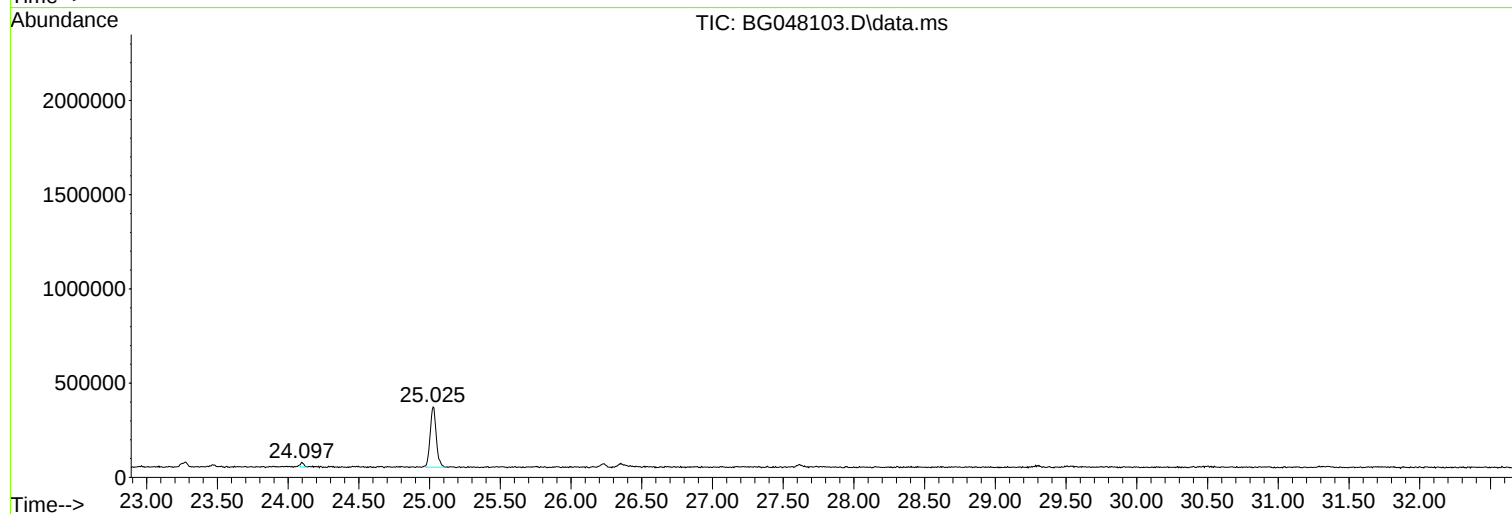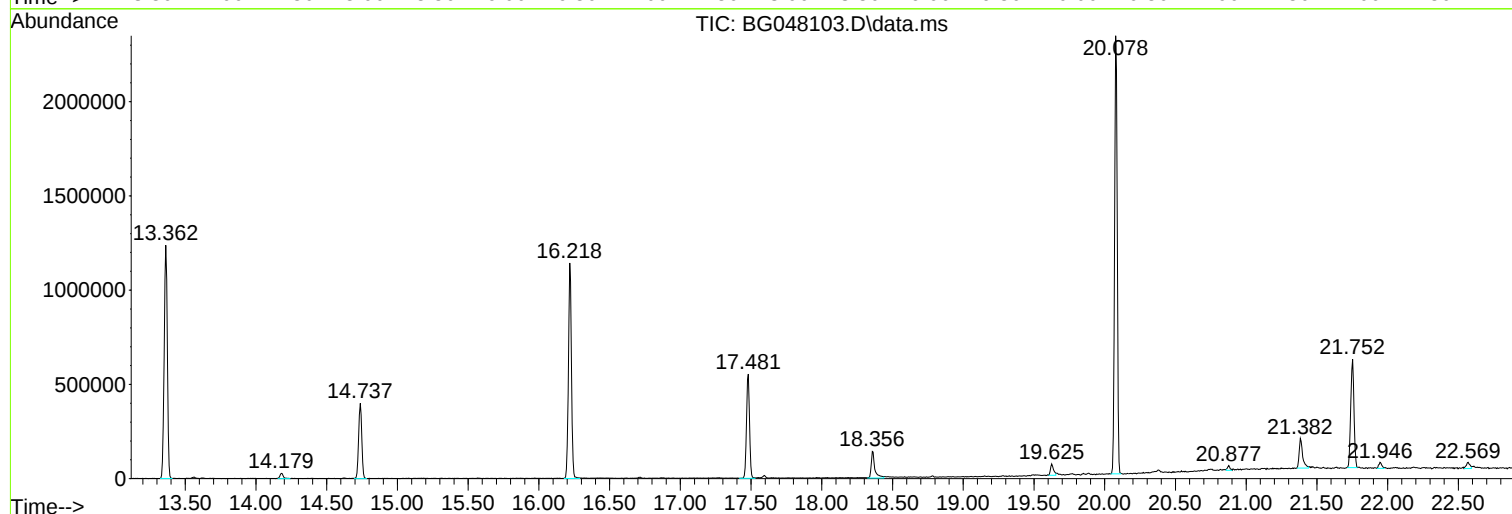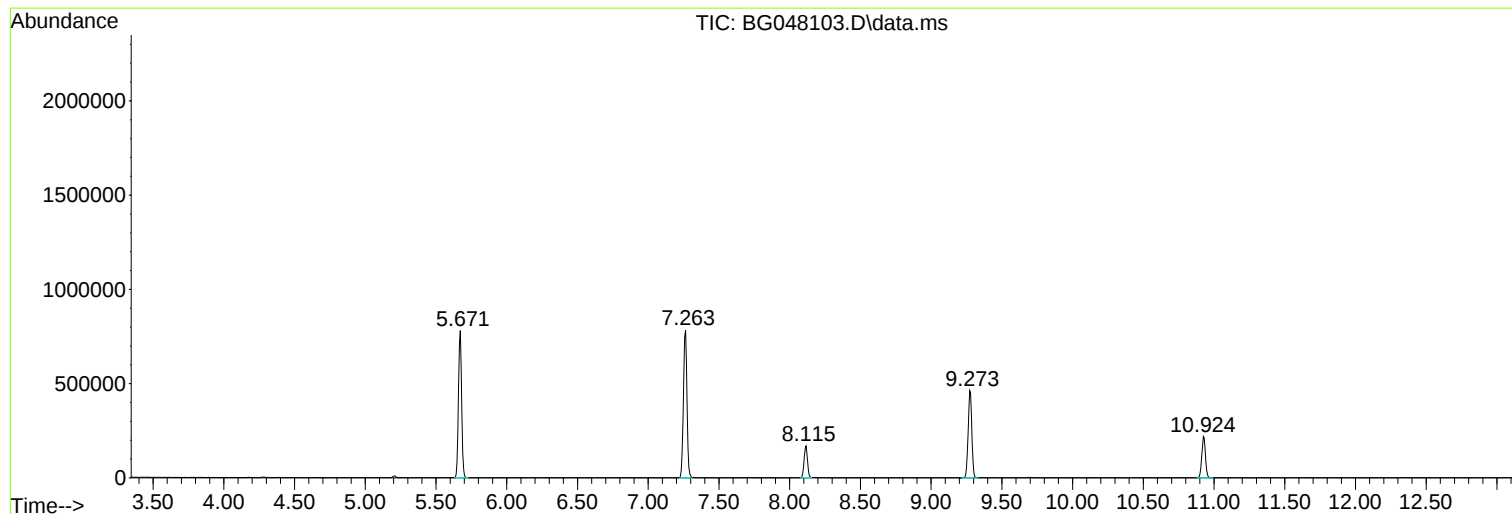

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048103.D
Acq On : 3 Feb 2021 22:59
Operator : CG/JU
Sample : M1291-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU421-007-1015

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048103.D
Acq On : 3 Feb 2021 22:59
Operator : CG/JU
Sample : M1291-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU421-007-1015

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
